

Manufactured for Immuno-Biological Laboratories Inc.
(IBL-America)
8201 Central Avenue, NE, Suite P
Minneapolis, MN 55432
Tel: 763-780-2955
Toll Free: 1-888-523-1246



Current Version Nr.: V 142.6

Previous Version: V 124.5

Update in section: General Update

Francisella tularensis IgG/IgM ELISA

CONTENTS

- 1 INTENDED USE
- 2 BACKGROUND
- 3 TEST PRINCIPLE
- 4 KIT COMPONENTS
- 5 MATERIAL REQUIRED BUT NOT SUPPLIED
- 6 STORAGE AND STABILITY
- 7 TEST PROCEDURE

**For Research Use
Only – Not for Use
in Clinical
Procedures**

- 7.1 General Information Evidence of Deterioration
- 7.2 Sample Preparation and Storage
- 7.3 Preparation of Kit Reagents
- 7.4 Overview - Test Procedure
- 7.5 Manual Test Procedure
- 7.6 Automated Test Procedure

8 TEST EVALUATION

- 8.1 Criteria of Validity
- 8.2 Cut-off Calculation
- 8.3 Interpretation of Results

9 PERFORMANCE CHARACTERISTICS

- 9.1 Sensitivity and Specificity
- 9.2 Reproducibility
- 9.3 Cross-Reactivities
- 9.4 Interfering Substances

10 SAFETY MEASURES

- 10.1 Statements of Warning
- 10.2 Disposal

11 REFERENCES

IBL-America Francisella tularensis IgG/IgM ELISA

Enzyme-immunoassay for determination of human antibodies

Francisella tularensis IgG ELISA

Order no.: IB05058

Francisella tularensis IgM ELISA

Order no.: IB05059

For Research Use Only – Not for Use in Clinical Procedures

1 INTENDED USE

The IBL-America ELISA Francisella tularensis IgG and IgM tests are qualitative immunoassays for the detection of human antibodies in serum or plasma directed against the lipopolysaccharide (LPS) of *Francisella tularensis*. These assays are recommended for the sensitive detection of such antibodies in various kinds of samples. These kits are for research use only.

2 BACKGROUND

Tularemia is a zoonosis caused by the *Francisella tularensis* bacterium and which can manifest in a variety of clinical conditions. Since the condition in animals resembles that of plague and the disease often affects hares and wild rabbits, it is also called rodent plague. Other traditional names for it are rabbit fever, lemming fever or Parinaud's disease.

Francisella tularensis (formerly also called *Pasteurella tularensis*) is a gram-negative pleomorphic bacterium. The three relevant forms of the four subspecies are difficult to differentiate. Two types can be distinguished epidemiologically, biochemically and genotypically: *Francisella tularensis* biovar *tularensis* (type A) is highly virulent and, untreated, the infection has a high mortality rate. *Francisella tularensis* biovar *holarctica* (type B) is much less virulent but can also cause severe illness.

Various small mammals, such as hares, rabbits, mice, rats and squirrels, are natural reservoirs of *Francisella tularensis*. The pathogen has also been detected in soil samples and water courses and can survive there for a prolonged period depending on climatic conditions. Human infection can occur through direct skin and mucosal contact with infected animals or their excreta. Extoparasites can also be considered as vectors. Consumption of infected and insufficiently cooked meat and inhalation of infectious dust are also potential routes of infection.

ELISA test-systems are especially suited for the differential analysis of immunoglobulin classes directed against the virus.

3 TEST PRINCIPLE

The ELISA (Enzyme Linked Immunosorbent Assay) is an immunoassay, which is particularly suited to the determination of antibodies in various kinds of samples. The reaction is based on the specific interaction of antibodies with their corresponding antigen. The test strips of the microtiter plate are coated with specific antigens of the pathogen of interest. If antibodies in the sample are present, they bind to the fixed antigen. A secondary antibody, which has been conjugated with the enzyme alkaline phosphatase, detects and binds to the immune complex. The colourless substrate p-nitrophenylphosphate is then converted into the coloured product p-nitrophenol. The signal intensity of this reaction product is proportional to the concentration of the analyte in the sample and is measured photometrically.

4 KIT COMPONENTS

| Test Components | Pieces / Volume |
|--|-----------------|
| Break apart microtiter test strips each with eight antigen coated single wells, (altogether 96) MTP , 1 frame. The coating material is inactivated. | 12 pieces |
| Standard serum (ready-to-use) STD , Human serum in protein containing phosphate buffer; negative for anti-HIV Ab, HBs-Ag (Hepatitis B-Virus surface antigen) and anti-HCV Ab; preservative: < 0.1 % sodium azide; colouring: Amaranth O. | 2 x 2 ml |
| Negative control serum (ready-to-use) NEG , Human serum in protein containing phosphate buffer; negative for anti-HIV Ab, HBs-Ag (Hepatitis B-Virus surface antigen) and anti-HCV Ab; preservative: < 0.1 % sodium azide; colouring: Lissamin Green V. | 2 ml |
| Anti-human IgG or IgM conjugate (ready-to-use) APC , Anti-human IgG or IgM polyclonal antibody, conjugated to alkaline phosphatase, stabilised with protein stabilisation solution; preservative: <0.1% methylisothiazolone, <0.1 % bromnitrodioxane. | 13 ml |
| Washing solution concentrate (sufficient for 1000 ml) WASH , Sodium chloride solution with Tween 20 and 30 mM Tris/HCl, pH 7,4; preservative: < 0.1 % sodium azide. | 33.3 ml |
| Dilution buffer DILB , Protein containing phosphate buffer with Tween 20; preservative: < 0.1 % sodium azide; colouring: 0.01 g/l Bromphenol blue. | 2 x 50 ml |
| Stopping solution STOP , <0.1 N sodium hydroxide, 40 mM EDTA | 15 ml |
| Substrate (ready-to-use) pNPP , Para-nitrophenylphosphate in solvent free buffer; preservative: < 0.1 % sodium azide | 13 ml |
| Quality control certificate INFO . | 1 page |

5 MATERIAL REQUIRED BUT NOT SUPPLIED

- common laboratory equipment
- for the IgM detection: Rf-Absorbent, order no. IB05998 (20 ml)
- photometer for microtitre plates with filter, wavelength 405 nm,
recommended reference wavelength 620 nm - 690 nm (e.g. 650 nm)
- incubator 37 °C
- moist chamber
- distilled water

6 STORAGE AND STABILITY

| Reagent | Storage | Stability |
|--|--|--|
| Microtiter strips (coated with antigen) | unopened after opening at 2 – 8 °C in closed aluminum bag with desiccant | see expiry date; minimum shelf-life: four weeks; |
| Control sera / Standard sera | Unopened after opening at 2 – 8 °C | see expiry date 6 months |
| Conjugate | Unopened after opening at 2 – 8 °C | see expiry date 6 months |
| Dilution buffer | Unopened after opening at 2 – 8 °C | see expiry date 6 months |
| Washing solution | Unopened / after opening at 2 – 8 °C working dilution at 2 – 8 °C working dilution at room temperature | see expiry date; 2 weeks; 1 week |
| Substrate | Unopened after opening at 2 – 8 °C | see expiry date 6 months |
| Stopping solution | Unopened after opening at 2 – 8 °C | see expiry date 6 months |

7 TEST PROCEDURE

7.1 General Information Evidence of Deterioration

Optimum results can only be achieved if the instructions are strictly followed. The components of the kit must not be exchanged for reagents of other manufacturers. Standard and control sera are defined exclusively for the test kit to be used and must not be used in other lots. Washing solution, substrate and stop solution can be used for all IBL-America immunoassays coded IB05xxx irrespective of the lot and the test.

Each test contains a ready-to-use sample dilution buffer. In some cases the use of special dilution buffers is necessary to guarantee consistent quality and reliable results. The dilution buffers can be used irrespective of the lots.

There are three different conjugate concentrations for each immunoglobulin class (IgA, IgG, IgM), indicated on the C of A as + (low), ++ (medium) and +++ (high). Conjugates

with the same concentration and of the same immunoglobulin class are interchangeable and can be used for other IB05xxx immunoassays irrespective of the lot and the test. Dilution or alteration of the reagents may result in a loss of sensitivity. Use aseptic techniques when removing aliquots from the reagent tubes to avoid contamination.

Reproducibility of test results is dependent on thorough mixing of the reagents. Agitate the flasks containing control sera before use and also all samples after dilution (e.g. by using a vortex mixer).

Be sure to pipette carefully and comply with the given incubation times and temperatures. Significant time differences between pipetting the first and last well of the microtiter plate when dispensing samples and control sera, conjugate or substrate can result in different pre-incubation times, which may influence the precision and reproducibility of the results. Avoid exposure of reagents to strong light during storage and incubation.

Adequate washing avoids test unspecificities. Therefore, the washing procedure should be carried out carefully. All of the flat bottom wells should be filled with equal volumes of washing buffer. At the end of the procedure ensure that the wells are free of all washing buffer in order to avoid uncontrolled dilution effects. Avoid foaming!

Reagents must be tightly closed after use to avoid evaporation and contamination. Take care not to mix-up the caps of the bottles and/or vials.

The immunoassay is only valid if the lot-specific validation criteria on the quality control certificate are fulfilled.

7.2 Sample Preparation and Storage

Lipaemic, hemolytic or icteric samples (serum or plasma) should only be tested with caution. Obviously contaminated samples should not be tested. Serum or plasma (EDTA, citrate, heparin) collected according to standard laboratory methods are suitable samples. Samples must not be thermally inactivated.

7.2.1 Dilution of Samples

Before running the test, all samples (V_1) must be diluted in dilution buffer (V_2) as follows:

Francisella tularensis IgG ELISA:

| | | |
|---------------------|----------------|---|
| $V_1 + V_2 = 1+100$ | add to each | 10 µl sample 1000 µl dilution buffer |
|---------------------|----------------|---|

After dilution and before pipetting into the microtiter plate the samples must be mixed thoroughly to prepare a homogenous solution.

Francisella tularensis IgM ELISA:

Interference with rheumatoid factors

Rheumatoid factors are autoantibodies mainly of the IgM class, which preferably bind to IgG immune complexes. The presence of non-specific IgM antibodies (rheumatoid factors) can lead to false-positive results in the IgM assay. Furthermore, the possibility exists, that weak-binding pathogen-specific IgM antibodies may be displaced by stronger-binding IgG antibodies leading to a false negative IgM result. Therefore it is necessary to pretreat samples with rheumatoid factor-absorbens prior to IgM detection (Rf-Absorbent). Rf-absorption is performed by incubation of the sample in Rf-dilution buffer for 15 minutes at room temperature or over night at 4 °C. The test procedure is described in a separate instruction manual.

Before running the test, rheumatoid factor-absorbent (V_1) must be diluted 1+4 in dilution buffer (V_2).

| | | |
|---------------------------------|----------------|---|
| $V_1 + V_2 = V_3 \text{ (1+4)}$ | add to each | 200 µl Rf absorbent 800 µl dilution buffer |
|---------------------------------|----------------|---|

Samples (V_4) must be diluted in this Rf-dilution buffer (V_3):

| | | |
|---------------------|----------------|---|
| $V_4 + V_3 = 1+100$ | add to each | 10 µl sample 1000 µl dilution buffer |
|---------------------|----------------|---|

After dilution and before pipetting into the microtiter plate the samples must be mixed thoroughly to prepare a homogenous solution.

7.2.2 Sample Storage

The samples should not be stored for more than 7 days at 2 – 8 °C. Extended storage is possible at ≤ -20 °C. Avoid repeated freezing and thawing of samples. Diluted samples can be stored at 2 – 8 °C for one week.

7.3 Preparation of Kit Reagents

Bring all reagents to room temperature before testing.

7.3.1 Microtiter Test Strips

The microtiter test strips labeled with abbreviations for pathogen and immunoglobulin class are packed with a desiccant in an aluminum bag. To open the aluminum bag of the microtiter plate please cut off the top of the marked side only, in order to guarantee proper resealing. Take unrequired cavities out of the frame and put them back into the aluminum bag. Close bag carefully to ensure airtight conditions. Do not use the strips if the aluminum bag is damaged or if the bag with remaining strips and desiccant was not properly resealed.

7.3.2 Negative control Sera / Standard Sera (ready-to-use)

Negative control and standard sera are ready-to-use and must not be diluted any further. For each test run (independent of the number of microtiter test strips to be used) negative control and standard sera must be included. Standard sera should be set up in duplicate. Do not treat negative control and standard sera with Rf-absorbent.

7.3.3 Anti-human IgG or IgM AP-Conjugate (ready-to-use)

The required conjugate concentration (+, ++, +++) is indicated on the quality control certificate. Avoid contamination.

7.3.4 Washing Solution

Dilute washing buffer concentrate (V_1) 1:30 with aqua dest. to a final volume of V_2 . Bottles used for the working dilution should be cleaned regularly. Discard cloudy solutions.

Example:

| Buffer concentrate (V_1) | Final volume (V_2) |
|------------------------------|------------------------|
| 33.3 ml | 1000 ml |
| 1.0 ml | 30 ml |

7.3.5 Dilution Buffer for Samples (ready-to-use)

Discard cloudy solutions.

7.3.6 Substrate (ready-to-use)

Substrate in unopened bottle may have a slightly yellow coloring, which does not reduce the quality of the product! Avoid contamination of the ready-to-use substrate solution e. g. by using sterile tips.

7.3.7 Stopping Solution (ready-to-use)


7.4 Overview - Test Procedure

IBL-America *Francisella tularensis IgG / IgM*

In case of IgM detection absorption of rheumatoid factor, see No. 7.2.1;
Incubation 15 minutes at room temperature or over night at 4°C

sample dilution¹
(samples)
1+100

Pipette diluted samples and ready-to-use negative control /
standard sera into the microtest wells (100 µl)

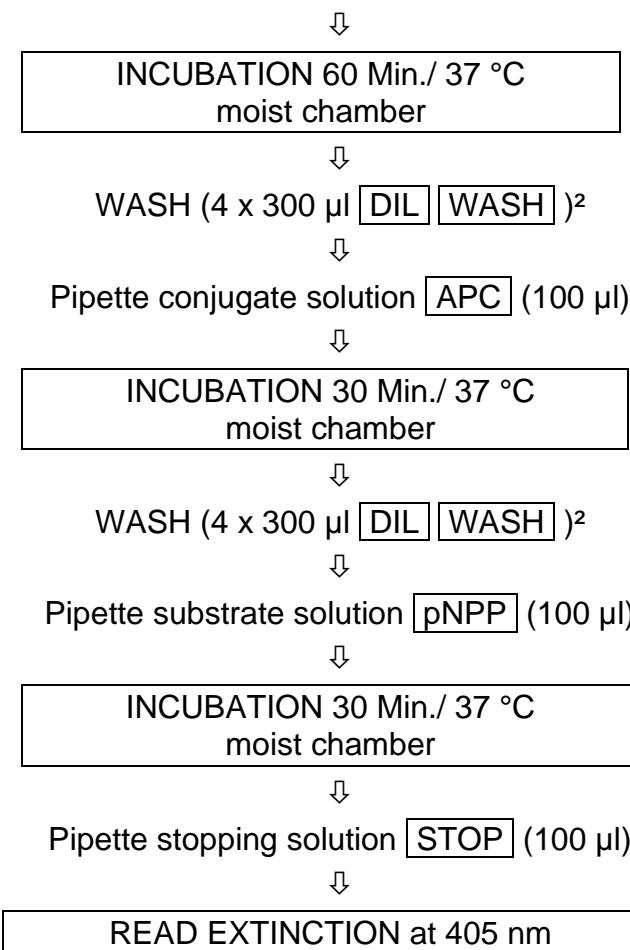

¹Special dilution buffers for the following IBL-America tests:
Borrelia burgdorferi IgG, IgM and EBV EA IgG

²For manual use:
tap plate at the end of the wash procedure on paper towel.

7.5 Manual Test Procedure

1. Place the required number of **cavities in the frame** and prepare a protocol sheet.
2. Add each **100 µl of diluted sample or ready-to-use negative control/standard sera** into the appropriate wells of microtiter test strips. Spare one well for substrate blank, e.g.:

| IgG/IgM | |
|----------|------------------|
| well no. | |
| well A1 | Substrate blank |
| well B1 | Negative Control |
| well C1 | Standard serum |
| well D1 | Standard serum |
| well E1 | Sample 1.... |
| well F1 | Sample 2.... |

3. **Sample incubation** for 60 minutes (+/- 5 min) at 37 °C (+/- 1 °C) in moist chamber
4. After incubation **wash** all wells with washing solution (by automated washer or manually):
 - aspirate or shake out the incubation solution
 - fill each well with 300 µl washing solution
 - aspirate or shake out the washing buffer
 - repeat the washing procedure 3 times (altogether 4 times!)
 - dry by tapping the microtiter plate on a paper towel
5. **Addition of conjugate**
Add 100 µl of the ready-to-use IgG/IgM conjugate to the appropriate wells (except substrate blank)
6. **Conjugate incubation** for 30 minutes (+/- 1 min)* at 37 °C (+/- 1 °C) in moist chamber.
7. After incubation **wash** all wells with washing solution (see above)
8. **Addition of substrate**
Add 100 µl of ready-to-use substrate solution to each well (including well for substrate blank!)
9. **Substrate incubation** for 30 minutes (+/- 1 min) at 37 °C (+/- 1 °C) in moist chamber.
10. **Stopping of the reaction**
Add 100 µl stopping solution to each well, shake microtiter plate gently to mix.
11. **Read extinction**
Read optical desity (OD) within 60 minutes at 405 nm against substrate blank, reference wave length between 620 nm and 690 nm (e.g. 650 nm).

7.6 Automated Test Procedure

This ELISA also is suited for processing on automats and evaluated for use with Immunomat™ (using the following consumables: VT124, VT111, VT112) and suited for processing on similar analyzers. For processing on the Immunomat the current software version including reagent check has to be used. The automated processing is performed analogous to manual use. Please note, that under special working-conditions internal laboratory adaptations of the substrate incubation times may be necessary.

8 TEST EVALUATION

For qualitative interpretation of serum samples a lot specific correction factor as well as a lot specific grey zone is calculated by manufacturer for each kit lot. These values can be found on the lot specific quality certificate included in each test kit.

For test run control a standard serum is used in each individual test run. For this control serum a reference value with a validity range is determined by the quality control of the manufacturer. Within this range a correct cut-off interpretation is ensured.

8.1 Criteria of Validity

The substrate blank must be < 0.25 OD

The negative control must produce a negative test result.

The mean OD-value (after subtraction of the substrate blank!) of the standard serum must be within the validity range, which is given on the lot specific quality control certificate.

The variation of OD-values of the standard serum may not be higher than 20%.

If these criteria are not met, the test is not valid and must be repeated.

8.2 Cut-off Calculation

A lot specific quality control certificate is included in the test kit so that the obtained OD values can be interpreted qualitatively. The substrate blank must be subtracted from all OD values prior to evaluation. Mean OD value of the standard serum (STD), tested in duplicate, has to be used. Mean OD value of the standard serum (STD), tested in duplicate, has to be used.

To fix the cut-off ranges multiply the mean value of the measured standard OD with the lot specific correction factor from the quality certificate. Then add and subtract the lot specific grey zone percentage mentioned on the quality certificate to obtain the upper and lower cut-off. The following numbers are an example only, the valid data you will find in the lot-specific QC certificate which comes with each kit.

Lot specific correction factor: 0.805

Lot specific grey zone: 15%

If the measured mean absorbance value of the standard serum is 0.84 OD, the range of the cut-off is:

Lower cut-off: $(0.84 * 0.805) - 15\% = \text{OD } 0,575$

Upper cut-off: $(0.84 * 0.805) + 15\% = \text{OD } 0,778$

8.3 Interpretation of Results

A positive test result confirms the presence of specific antibodies. A negative result indicates that no relevant antibodies against the pathogen are present in the sample, but does not exclude the possibility of an acute reaction. In case of a borderline result a reliable evaluation is not possible. A definitive determination can only be achieved by testing paired serum samples, taken at one to two weeks intervals, in parallel.

The borderline range indicates the range for borderline test results. Values obtained, when testing a sample, which fall below this range indicate a negative test result; values above the borderline range are interpreted positive.

A negative result in the Francisella tularensis assay indicates that there are no antibodies in the serum to the lipopolysaccharide of the pathogen. In the case of a borderline result, the test should be repeated in parallel with a new sample taken after an interval of one to two weeks (paired sera). A positive result confirms the presence of LPSspecific antibodies.

9 PEFORMANCE CHARACTERISTICS

9.1 Sensitivity and Specificity

IBL-America Francisella tularensis IgG and IgM

The IBL-America Francisella tularensis IgG and IgM ELISA were verified in an internal study.

| | Sensitivity | Specificity |
|---|-------------|-------------|
| SERION ELISA classic Francisella tularensis IgG | > 99 % | 99.0 % |
| SERION ELISA classic Francisella tularensis IgM | > 99 % | 96.4 % |

9.2 Reproducibility

Francisella tularensis IgG:

| Sample | Mean Value (OD) | Intraassay (CV %) | Mean Value (OD) | Interassay (CV %) |
|---------|--------------------|----------------------|--------------------|----------------------|
| Serum 1 | 0.810 | 3.4 | 0.860 | 6.3 |
| Serum 2 | 1.153 | 2.1 | 1.239 | 8.4 |
| Serum 3 | 1.898 | 2.7 | 2.007 | 3.6 |

Francisella tularensis IgM:

| Sample | Mean Value (OD) | Intraassay (CV %) | Mean Value (OD) | Interassay (CV %) |
|---------|--------------------|----------------------|--------------------|----------------------|
| Serum 1 | 0.445 | 7.4 | 0.574 | 8.2 |
| Serum 2 | 0.604 | 5.9 | 0.607 | 9.2 |
| Serum 3 | 1.307 | 4.4 | 1.219 | 7.9 |

9.3 Cross-Reactivities

Francisella tularensis IgG

To determine detection of cross-reactive antibodies directed against different parameters sera were analyzed with the Francisella tularensis IgG ELISA and a commercially available anti-Francisella tularensis ELISA. Positive sera (10 sera each) for Yersinia IgG, Cytomegalovirus IgG, Toxoplasma gondii IgG and Epstein-Barr Virus VCA IgG have been tested as well as sera positive for rheumatoid factor (RF) and anti-nuclear antibodies (ANA). Within this internal evaluation potential cross-reactivities with one ANA positive serum has been observed. All reactivities have been confirmed by positive or borderline results in the reference assay. Other cross-reactivities cannot be ruled out in general.

Francisella tularensis IgM

To determine detection of cross-reactive antibodies directed against different parameters sera were analyzed with the Francisella tularensis IgM ELISA and a commercially available anti-Francisella tularensis ELISA. Positive sera (10 sera each) for Yersinia IgM, Cytomegalovirus IgM, Toxoplasma gondii IgM and Epstein-Barr Virus VCA IgM have been tested as well as sera positive for rheumatoid factor (RF) and anti-nuclear antibodies (ANA). Within this internal evaluation no potential cross-reactivities have been observed. Other cross-reactivities cannot be ruled out in general.

9.4 Interfering Substances

Francisella tularensis IgG/IgM

To determine the influence of interfering substances, sera with different reactivities were analyzed with the Francisella tularensis IgG/IgM ELISAs. No interferences have been detected for sera with concentrations up to 2.00 g/L hemoglobin, 11.50 g/L lipemia/triglyceride or 0.201 g/L bilirubin (conjugated and unconjugated).

10 SAFETY MEASURES

10.1 Statements of Warning

The IBL-America ELISA test kits are designed for use by qualified personnel who are familiar with good laboratory practice.

All kit reagents and human specimens should be handled carefully, using established good laboratory practice.

- This kit contains human blood components. Although all control- and cut-off sera have been tested and found negative for anti-HIV-ab, HBs-Ag (*Hepatitis B-Virus-surface Antigen*) and anti-HCV-ab, they should be considered potentially infectious.
- Do not pipette by mouth.
- Do not smoke, eat or drink in areas in which specimens or kit reagents are handled.
- Wear disposable gloves, laboratory coat and safety glasses while handling kit reagents or specimens. Wash hands thoroughly afterwards.
- Sample material and other potentially infectious material should be decontaminated after the test run.
- Reagents should be stored safely and be inaccessible to unauthorized access e.g. children.

10.2 Disposal

Please observe the relevant statutory requirements!

11 REFERENCES

- [1] Ellis, J., Oyston, P.C.F., Green, M., Titball, R.W. (2002) Tularemia. Clin. Microbiol. Rev. 15, 631-46.
- [2] Fritzsch, J., Splettstoesser, WD. (2010) Septic pneumonic tularaemia caused by Francisella tularensis subsp. holarctica biovar II. J. Med. Microbiol. 59, 1123 – 5.
- [3] Grunow, R., Splettstößer, W., Hirsch, F.W., Kleemann, D., Finke, E.-J. (2001) Differentialdiagnose der Tularämie. Dtsch. Med. Wschr. 126, 408-13.
- [4] Haristoy, X., Lozniewski, A., Tram, C., Simeon, D., Bevanger, L., Lion, C. (2003) Case Reports Francisella tularensis bacteremia. J. Clin. Microbiol. 41, 2774-6.
- [5] Svensson, K., Larsson, P., Johansson, D., Byström, M., Forsman, M., Johansson, A. (2005) Evolution of subspecies of Francisella tularensis. J. Bacteriol. 187, 3903-8.
- [6] Yeşilyurt, M., Kılıç, S., Çelebi, B., Gül, S. (2013) Tularemia during pregnancy: Report of four cases. Scand. J. Infect. Dis. 45, 324 – 8.

Manufactured for Immuno-Biological Laboratories Inc.
(IBL-America)
8201 Central Avenue, NE, Suite P
Minneapolis, MN 55432
Tel: 763-780-2955
Toll Free: 1-888-523-1246

