

# Product information

Information about other products is available at [www.ibl-america.com](http://www.ibl-america.com)



## User's Manual

# Human FGF2 ELISA

## (Heparin-binding growth factor 2)

Enzyme immunoassay for detection of Human FGF2 in serum, plasma, tissue homogenates and other biological fluids.

**REF**

**IB08011**



**96 wells**

**RUO**

**For Research Use Only – Not for Use in Diagnostic Procedures**

## 1 INTRODUCTION

### 1.1 Intended Use

The Human Heparin-binding growth factor 2 (FGF2) ELISA has been designed for the detection of FGF2 in serum, plasma, tissue homogenates and other biological fluids. For research use only, not for use in diagnostic procedures.

## 2 PRINCIPLE OF THE TEST

This kit is based on sandwich enzyme-linked immune-sorbent assay technology. Capture antibody is pre-coated onto 96-well plates. And the biotin conjugated antibody is used as detection antibodies. The standards, test samples and biotin conjugated detection antibody are added to the wells subsequently, and washed with wash buffer. HRP-Streptavidin is added and unbound conjugates are washed away with wash buffer. TMB substrates are used to visualize HRP enzymatic reaction. TMB is catalyzed by HRP to produce a blue color product that changed into yellow after adding acidic stop solution. The density of yellow is proportional to the target amount of sample captured in plate. Read the O.D. absorbance at 450nm in a microplate reader, and then the concentration of target can be calculated.

## 3 WARNINGS AND PRECAUTIONS

1. To inspect the validity of experiment operation and the appropriateness of sample dilution proportion, pilot experiment using standards and a small number of samples is recommended.
2. After opening and before using, keep plate dry.
3. Before using the Kit, spin tubes and bring down all components to the bottom of tubes.
4. Storage TMB reagents avoid light.
5. Washing process is very important, not fully wash easily cause a false positive and high background.
6. Duplicate well assay is recommended for both standard and sample testing.
7. Don't let Micro plate dry at the assay, for dry plate will inactivate active components on plate.
8. Don't reuse tips and tubes to avoid cross contamination.
9. Avoid using the reagents from different batches together.

## 4 Reagents

### 4.1 Reagents provided

1. ELISA Microplate(Dismountable)
2. Lyophilized Standard: 2 vials
3. Sample/Standard Dilution Buffer: 20 ml
4. Biotin-labeled Antibody (Concentrated): 120  $\mu$ l
5. Antibody Dilution Buffer: 10 ml
6. HRP-Streptavidin Conjugate(SABC): 120  $\mu$ l Protect from Light
7. SABC Dilution Buffer: 10 ml
8. TMB Substrate: 10 ml Protect from Light
9. Stop solution: 10 ml
10. Wash Buffer (25X): 30 ml
11. Plate Sealer: 5 pieces
12. Product Description: 1 copy

### 4.2 Materials required but not provided

1. Microplate reader (wavelength:450nm)
2. 37°C incubator
3. Automated plate washer
4. Precision single and multi-channel pipette and disposable tips
5. Clean tubes and Eppendorf tubes
6. Deionized or distilled water

### 4.3 Storage Conditions / Expiration

Store at 4°C for 6 months

#### 4.4 Washing Procedure

**Manual:** Discard the solution in the plate without touching the side walls. Clap the plate on absorbent filter papers or other absorbent material. Fill each well completely with 350ul wash buffer and soak for 1 to 2 minutes, then aspirate contents from the plate, and clap the plate on absorbent filter papers or other absorbent material.

**Automatic:** Aspirate all wells, and then wash plate with 350ul wash buffer. After the final wash, invert plate, and clap the plate on absorbent filter papers or other absorbent material. It is recommended that the washer shall be set for soaking 1 minute. (**Note:** set the height of the needles; be sure the fluid can be sipped up completely)

#### 4.5 Sample Collection and Storage (universal)

##### 1. Sample

- **Serum:** Place whole blood sample at room temperature for 2 hours or put it at 4°C overnight and centrifugation for 20 minutes at approximately 1000×g, Collect the supernatant and carry out the assay immediately. Blood collection tubes should be disposable, non-pyrogenic, and non-endotoxin.
- **Plasma:** Collect plasma using (EDTA-Na<sub>2</sub> or heparin as an anticoagulant. Centrifuge samples for 15 minutes at 1000×g at 2 - 8°C within 30 minutes of collection. Collect the supernatant and carry out the assay immediately. Avoid hemolysis, high cholesterol samples.
- **Tissue Homogenates:** As hemolysis blood has relation to assay result, it is necessary to remove residual blood by washing tissue with pre-cooling PBS buffer (0.01M, pH=7.4). Mince tissue after weighing it and get it homogenized in PBS (the volume depends on the weight of the tissue. Normal, 9mL PBS would be appropriate to 1 gram tissue pieces. Some protease inhibitors are recommended to add into the PBS) with a glass homogenizer on ice. To further break the cells, you can sonicate the suspension with an ultrasonic cell disrupter or subject it to freeze-thaw cycles. The homogenates are then centrifuged for 5minutes at 5000×g to get the supernatant. The total protein concentration was determined by BCA kit and the total protein concentration of each pore sample should not exceed 0.3mg.
- **Cell Culture Supernatant:** Centrifuge supernatant for 20 minutes at 1000×g at 2 - 8°C to remove insoluble impurity and cell debris. Collect the clear supernatant and carry out the assay immediately.
- **Cell Culture Lysate:** Commercial RIPA kits are recommended to follow the instructions provided. Generally, 0.5ml RIPA lysis buffer would be appropriate to 2×10<sup>6</sup>cells, DNA must to be removed. The total protein concentration was determined by BCA kit and the total protein concentration of each pore sample should not exceed 0.3mg.
- **Other Biological Fluids:** Centrifuge samples for 20 minutes at 1000×g at 2-8°C. Collect supernatant and carry out the assay immediately.

**Note:** Samples to be used within 5 days can be stored at 4°C, besides that, samples must be stored at -20°C (assay ≤1 month) or -80°C (assay ≤2 months) to avoid loss of bioactivity and contamination. Avoid multiple freeze-thaw cycles. The hemolytic samples are not suitable for this assay.

##### 2. Sample Dilution

The user should estimate the concentration of target protein in the test sample, and select a proper dilution factor to make the diluted target protein concentration fall in the optimal detection range of the kit. Dilute the sample with the provided dilution buffer, and several trials may be necessary. The test sample must be well mixed with the dilution buffer. And also standard curves and sample should be making in pre-experiment. If samples with very high concentrations, dilute samples with PBS first and then dilute the samples with Sample Dilution.

**The matrix components in the sample will affect the test results, which it need to be diluted at least 1/2 with Sample Dilution Buffer before testing!**

#### 4.6 Reagent Preparation and Storage

Bring all reagents and samples to room temperature for 20 minutes before use.

##### 1. Wash buffer

If crystals have formed in the concentrate, you can warm it with 40°C water bath (Heating temperature should not exceed 50°C) and mix it gently until the crystals have completely been dissolved. The solution should be cooled to room temperature before use.


Dilute 30ml (15ml for 48T) Concentrated Wash Buffer into 750ml (375ml for 48T) Wash Buffer with deionized or distilled water. Put unused solution back at 4°C.

## 2. Standards

1). Add 1 ml Sample Dilution Buffer into one Standard tube (labeled as zero tube), keep the tube at room temperature for 10 minutes and mix them thoroughly.

**Note: If the standard tube concentration is higher than the range of the kit , please dilute it and labeled as zero tube.**

2). Label 7 EP tubes with 1/2, 1/4, 1/8, 1/16, 1/32, 1/64 and blank respectively. Add 0.3ml of the Sample Dilution Buffer into each tube. Add 0.3ml of the above Standard solution (from zero tube) into 1st tube and mix them thoroughly. Transfer 0.3ml from 1st tube to 2nd tube and mix them thoroughly. Transfer 0.3ml from 2nd tube to 3rd tube and mix them thoroughly, and so on. Sample Dilution Buffer was used for the blank control.

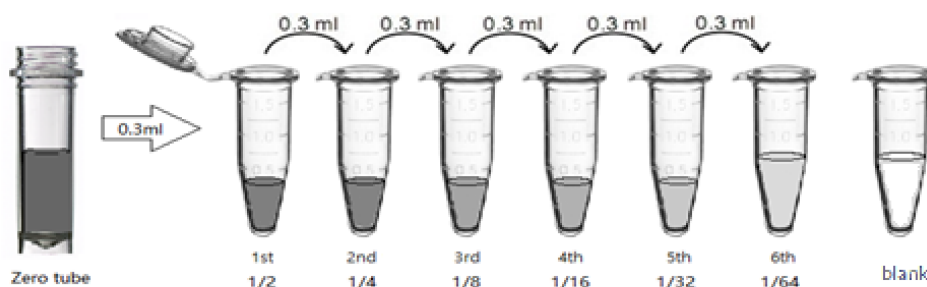

**Prepare standard solutions**

**Note:** It is best to use Standard Solutions within 2 hours.

## 3. Preparation of Biotin-labeled Antibody Working Solution

Prepare it within 1 hour before experiment.

- 1) Calculate required total volume of the working solution:  $0.1\text{ ml} / \text{well} \times \text{quantity of wells}$ . (Allow 0.1-0.2ml more than the total volume)
- 2) Dilute the Biotin-detection antibody with Antibody Dilution Buffer at 1:100 and mix them thoroughly. (i.e. Add  $1\ \mu\text{l}$  Biotin-labeled antibody into  $99\ \mu\text{l}$  Antibody Dilution Buffer.)

## 4. Preparation of HRP-Streptavidin Conjugate (SABC) Working Solution

Prepare it within 30 minutes before experiment.

- 1) Calculate required total volume of the working solution:  $0.1\text{ ml} / \text{well} \times \text{quantity of wells}$ . (Allow 0.1-0.2ml more than the total volume)
- 2) Dilute the SABC with SABC Dilution Buffer at 1:100 and mix them thoroughly. (i.e. Add  $1\ \mu\text{l}$  of SABC into  $99\ \mu\text{l}$  of SABC Dilution Buffer.)

## 5 ASSAY PROCEDURE

### 5.1 General Remarks

When diluting samples and reagents, they must be mixed completely and evenly. Before adding TMB into wells, equilibrate TMB Substrate for 30 min at 37 °C. It is recommended to plot a standard curve for each test.

### 5.2 Test Procedure


1. Set standard, **test samples (diluted at least 1/2 with Sample Dilution Buffer)**, control (blank) wells on the pre-coated plate respectively, and then, records their positions. It is recommended to measure each standard and sample in duplicate. **Wash plate 2 times before adding standard, sample and control (blank) wells!**
2. **Prepare Standards:** Aliquot 100µl of zero tube, 1<sup>st</sup>tube, 2<sup>nd</sup>tube, 3<sup>rd</sup>tube, 4<sup>th</sup>tube, 5<sup>th</sup>tube, 6<sup>th</sup>tube and Sample Dilution Buffer (blank) into the standard wells.
3. **Add Samples:** Add 100µl of properly diluted sample into test sample wells.
4. **Incubate:** Seal the plate with a cover and incubate at 37°C for 90 minutes.
5. **Wash:** Remove the cover and discard the plate content and wash plate 2 times with Wash Buffer. Do NOT let the wells dry completely at any time.
6. **Biotin-labeled Antibody:** Add 100µl Biotin-labeled antibody working solution into above wells (standard, test sample and blank wells). Add the solution at the bottom of each well without touching the sidewall, cover the plate and incubate at 37°C for 60 minutes.
7. **Wash:** Remove the cover, and wash plate 3 times with Wash Buffer, and let the Wash Buffer stay in the wells for 1-2 minute each time.
8. **HRP-Streptavidin Conjugate (SABC):** Add 100µl of SABC Working Solution into each well, cover the plate and incubate at 37°C for 30 minutes.
9. **Wash:** Remove the cover and wash plate 5 times with Wash Buffer and let the wash buffer stay in the wells for 1-2 minute each time.
10. **TMB Substrate:** Add 90µl TMB Substrate into each well, cover the plate and incubate at 37°C in dark within 10-20 minutes. (**Note:** The reaction time can be shortened or extended according to the actual color change, but not more than 30minutes. You can terminate the reaction when apparent gradient appeared in standard wells.)
11. **Stop:** Add 50µl Stop Solution into each well. The color will turn yellow immediately. The adding order of Stop Solution should be as the same as the TMB Substrate Solution.
12. **OD Measurement:** Read the O.D. absorbance at 450 nm in Microplate Reader immediately after adding the stop solution.

### 5.3 Results

Regarding calculation,  $(\text{the relative O.D.450}) = (\text{the O.D.450 of each well}) - (\text{the O.D.450 of blank well})$ . The standard curve can be plotted as the relative O.D.450 of each standard solution (Y) vs. the respective concentration of the standard solution (X). The target concentration of the samples can be interpolated from the standard curve. It is recommended to use some professional software to do this calculation, such as **Curve Expert 1.3 or 1.4.**

**Note:** If the samples measured were diluted, multiply the dilution factor to the concentrations from interpolation to obtain the concentration before dilution.

## 5.4 Summary

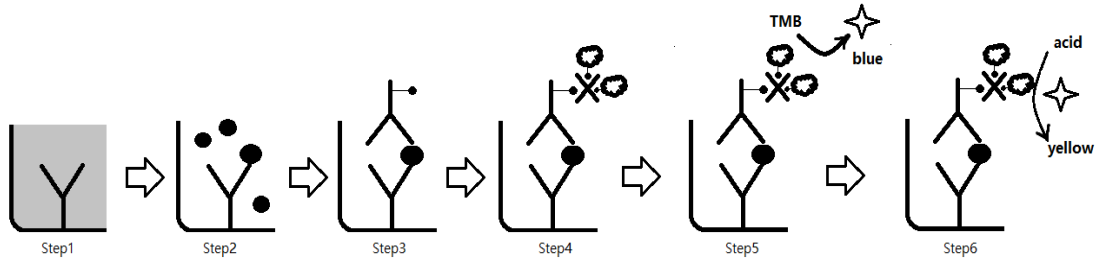

**Step1** : Wash plate 2 times before adding Standard, **Sample (diluted at least 1/2 with Sample Dilution Buffer)** and Control (blank) wells!

**Step2** : Add 100µl standard or sample to each well and incubate for 90 minutes at 37°C.

**Wash step** : Aspirate and wash plates 2 times.

**Step3** : Add 100µl Biotin-labeled antibody working solution to each well and incubate for 60 minutes at 37°C.

**Wash step** : Aspirate and wash plates 3 times.

**Step4** : Add 100µl SABC Working Solution into each well and incubate for 30 minutes at 37°C.

**Wash step** : Aspirate and wash plates 5 times.

**Step5** : Add 90µl TMB Substrate Solution. Incubate 10-20 minutes at 37°C.

**Step6** : Add 50µl Stop Solution. Read at 450nm immediately and calculation.

## 6 QUALITY CONTROL

Good laboratory practice requires that controls be run with each calibration curve. A statistically significant number of controls should be assayed to establish mean values and acceptable ranges to assure proper performance. It is recommended to use controls according to state and federal regulations. The use of controls is advised to assure the day to day validity of results. It is also recommended to make use of national or international Quality Assessment programs in order to ensure the accuracy of the results. Employ appropriate statistical methods for analyzing control values and trends. If the results of the assay do not fit to the established acceptable ranges of control materials, results of unknowns should be considered invalid.

In this case, please check the following technical areas: Pipetting and timing devices; photometer, expiration dates of reagents, storage and incubation conditions, aspiration and washing methods. After checking the above mentioned items without finding any error contact your distributor or IBL-America directly.

## 7 PERFORMANCE CHARACTERISTICS

### 7.1 Range

12.5 – 800 pg/mL


### 7.2 Sensitivity

7.5 pg/mL

### 7.3 Typical Data & Standard Curve

Results of a typical standard operation of a FGF2 ELISA Kit are listed below. This standard curve was generated at our lab for demonstration purpose only. Users shall obtain standard curve as per experiment by themselves. (N/A=not applicable)

STD.(pg/ml)	OD-1	OD-2	Average	Corrected
0	0.032	0.032	0.032	0.000
12.5	0.051	0.053	0.052	0.02
25	0.087	0.089	0.088	0.036
50	0.148	0.152	0.15	0.062
100	0.294	0.302	0.298	0.148
200	0.826	0.85	0.838	0.54
400	1.656	1.704	1.68	0.842
800	2.536	2.61	2.573	0.893

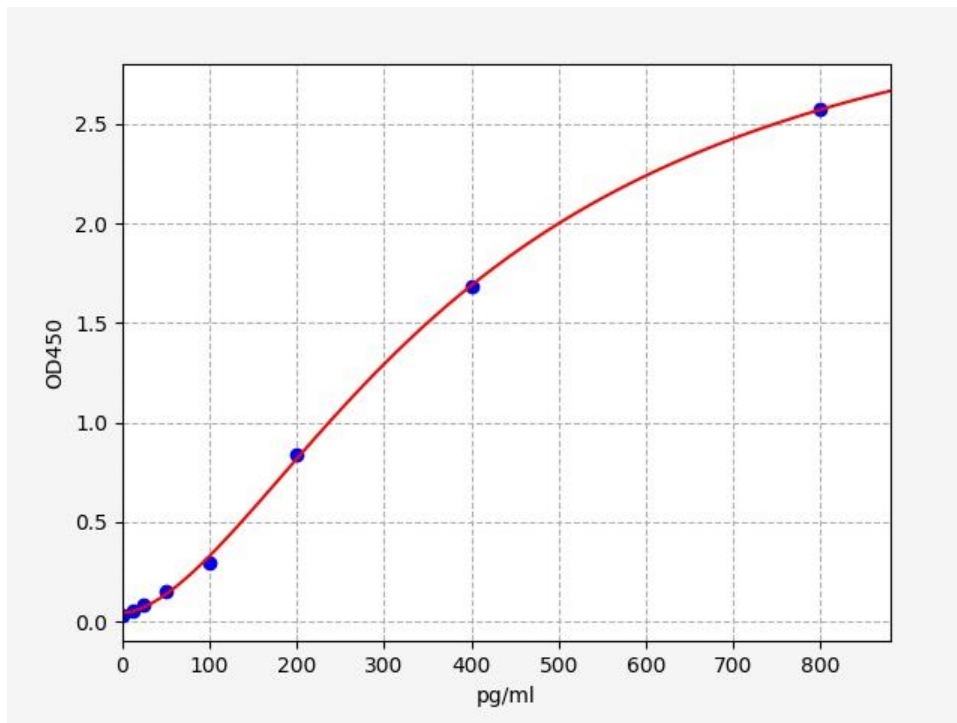

## 7.4 Specificity

This assay has high sensitivity and excellent specificity for detection of FGF2. No significant cross-reactivity or interference between FGF2 and analogues was observed.

Note: Limited by current skills and knowledge, it is difficult for us to complete the cross-reactivity detection between FGF2 and all the analogues, therefore, cross reaction may still exist.

## 7.5 Recovery

Matrices listed below were spiked with certain level of FGF2 and the recovery rates were calculated by comparing the measured value to the expected amount of FGF2 in samples.

Matrix	Recovery Range (%)	Average (%)
Serum(n=5)	88-92	90
EDTA Plasma(n=5)	88-105	95
Heparin Plasma(n=5)	91-104	97

## 7.6 Linearity

The linearity of the kit was assayed by testing samples spiked with appropriate concentration of FGF2 and their serial dilutions. The results were demonstrated by percentage of calculated concentration to the expectation.

Sample	1:2	1:4	1:8
Serum(n=5)	95-102%	89-102%	88-104%
EDTA Plasma(n=5)	86-99%	91-99%	87-101%
Heparin Plasma(n=5)	80-99%	81-96%	83-95%

## 7.7 Precision

Intra-Assay: CV<8%

Inter-Assay: CV<10%

## 7.8 Stability

The stability of ELISA kit is determined by the loss rate of activity. The loss rate of this kit is less than 10% within the expiration date under appropriate storage condition.

Standard (n=5)	37°C for 1 month	4°C for 6 months
Average (%)	80	95-100

To minimize extra influence on performance, operation procedures and lab conditions, especially room temperature, air humidity, incubator temperature should be strictly controlled. It is strongly suggested that the same operator performs the whole assay from the beginning to the end.



## **8 ORDERING INFORMATION**

This kit is manufactured for Immuno-Biological Laboratories, Inc. (IBL-America). For ordering information, please contact:

**Immuno-Biological Laboratories, Inc. (IBL-America)**

8201 Central Ave NE, Suite P

Minneapolis, MN 55432

Toll Free: (888) 523-1246

Fax: (763) 780-2988

[www.ibl-america.com](http://www.ibl-america.com)

[info@ibl-america.com](mailto:info@ibl-america.com)