



User's Manual

Rat Monocyte Chemoattractant Protein-1 (MCP-1) ELISA

Sandwich Enzyme-Linked Immunosorbent Assay for the detection
of Rat MCP-1

REF

IB99563



96

Storage: 2-8°C

RUO

For research use only, not for use in diagnostic procedures.

Contents

1. Introduction	3
2. Principles of Method	3
3. Intended Use	4
4. Storage and Stability	4
5. Chemical Hazard	4
6. Kit Contents	5
7. Materials Required But Not Provided	6
8. Reagent preparation	6
1) Rat MCP-1 standard	6
2) Secondary Antibody	6
3) Streptavidin- HRP	7
4) Washing buffer	7
5) Sample preparation	7
9. Assay Procedure	8
10. Characteristics	9
1) Typical result	9
2) Sensitivity	10
3) Specificity	10
4) Precision	11
5) Recovery	11
11. Troubleshooting	12
12. Reference	13

1. Introduction

The chemokine (C-C motif) ligand 2 (CCL2) is also referred to as monocyte chemoattractant protein 1 (MCP1) and small inducible cytokine A2. CCL2 is a small cytokine that belongs to the CC chemokine family. CCL2 recruits monocytes, memory T cells, and dendritic cells to the sites of inflammation produced by either tissue injury or infection. CCL2 is a monomeric polypeptide, with a molecular weight of approximately 13 kDa. CCL2 is anchored in the plasma membrane of endothelial cells by glycosaminoglycan side chains of proteoglycans. CCL2 is primarily secreted by monocytes, macrophages and dendritic cells. Platelet derived growth factor is a major inducer of CCL2 gene. To become activated CCL2 protein has to be cleaved by metalloproteinase MMP-12. CCL2 exhibits a chemotactic activity for monocytes and basophils. However, it does not attract neutrophils or eosinophils. After deletion of the N-terminal residue, CCL2 loses its attractivity for basophils and becomes a chemoattractant of eosinophils. Basophils and mast cells that are treated with CCL2 releases their granules to the intercellular space. This effect can be also potentiated by a pre-treatment with IL-3 or even by other cytokines. CCL2 augments monocyte anti-tumor activity and it is essential for formation of granulomas. The CCL2 chemokine is also expressed by neurons, astrocytes and microglia. The expression of CCL2 in neurons is mainly found in the cerebral cortex, globus pallidus, hippocampus, paraventricular and supraoptic hypothalamic nuclei, lateral hypothalamus, substantia nigra, facial nuclei, motor and spinal trigeminal nuclei, gigantocellular reticular nucleus and in Purkinje cells in the cerebellum.

2. Principles of Method

The design of this assay is based on a sandwich Enzyme-Linked Immunosorbent Assay (ELISA). The microtiter plate provided in this kit has been pre-coated with a monoclonal antibody specific to Rat MCP-1. Samples are pipetted into these wells. Nonbound Rat MCP-1 and other components of the sample should be removed by washing, then monoclonal antibody specific to Rat MCP-1 added. In order to quantitatively determine the amount of Rat MCP-1 present in the sample, Streptavidin Horseradish Peroxidase (HRP) should be added to each microplate well. The final step, a TMB-substrate solution added to each well. Finally, a sulfuric acid solution is added and the resulting yellow colored product is measured at 450nm. Since the increases in absorbency is directly proportional to the amount of captured Rat MCP-1.

3. Intended Use

The IBL-AMERICA Rat MCP-1 ELISA kit is to be used for the determination of Rat MCP-1 in Human serum, Human plasma, cell lysate, culture supernatants and buffered solution. The assay will recognize native and recombinant Rat MCP-1.

This kit has been configured for research use only and is not to be used in diagnostic procedures.

4. Storage and Stability

All kit components of this kit are stable at 2 to 8°C. Any unused reconstituted standard should be discarded or frozen at -70°C. Standard can be frozen and thawed one time only without loss of immunoreactivity.

5. Chemical Hazard

- Stop solution: This reagent is an irritant to eyes, skin and mucous membranes. Avoid contact with eyes, skin and clothing. Wear suitable protective clothing, gloves and eye protection. In the event of contact with eyes or skin, wash immediately with plenty of water.
- Standard protein and 2nd Antibody containing Sodium Azide as a preservative.

6. Kit Contents

Contents	Number	Volume
96 Well Plate	1 (in aluminum foil bag with desiccant)	
Washing Buffer	2	(20X) 25 ml
Standard Protein	1 Glass vial (lyophilized)	
Standard/Sample Dilution Buffer	1	25 ml
Secondary Antibody	1 Glass vial (lyophilized)	
Streptavidin HRP(X100)	1	150 μ l
Secondary antibody/ Streptavidin HRP Dilution Buffer	1	25 ml
Substrate (TMB)	1	15 ml
Stop Solution	1	15 ml
Protocol booklet	1	
Plate sealers	2	

- ① 96 Well Plate
: Rat MCP-1 microtiter plate, one plate of 96 wells (8 well strips x 12).
A plate using break-apart strips coated with a mouse monoclonal antibody specific to Rat MCP-1.
 - ② Standard Protein
: Recombinant Rat MCP-1.
 - ③ Secondary Antibody
: Biotinylated anti Rat MCP-1 antibody.
 - ④ Streptavidin HRP
: Streptavidin Horseradish Peroxidase (HRP, enzyme)
 - ⑤ Substrate (Stabilized chromogen)
: Tetramethylbenzidine (TMB) solution
 - ⑥ Stop Solution
: 1N solution of sulfuric acid (H₂SO₄).
 - ⑦ Plate sealer
: Adhesive sheet.
- Do not mix or interchange different reagents from various kit lots.

7. Materials Required But Not Provided

- ① Microtiter plate reader capable of measurement at or near 450nm.
- ② Calibrated, adjustable precision pipettes, preferably with disposable plastic tips (A manifold multi-channel pipette is desirable for large assays.)
- ③ Distilled or deionized water
- ④ Data analysis and graphing software
- ⑤ Vortex mixer
- ⑥ Polypropylene tubes for diluting and aliquoting standard
- ⑦ Absorbent paper towels
- ⑧ Calibrated beakers and graduated cylinders of various sizes

8. Reagent Preparation

1) Rat MCP-1 standard

1. Reconstitute the lyophilized Rat MCP-1 standard by adding 1.0 ml of *Standard/Sample Dilution Buffer* to make the 5 ng/ml standard stock solution. Allow solution to sit at RT for 5 minutes, then gently vortex to mix completely. Use within one hour of reconstituting
2. Prepare 1 ml of 1000 pg/ml top standard by adding 200 μ l of the above stock solution in 800 μ l of *Standard/Sample Dilution Buffer*. Perform 2-fold serial dilutions of the top standards to make the standard curve within the range of this assay (15.625 pg/ml ~ 1000 pg/ml) as below. *Standard/Sample Dilution Buffer* serves as the zero standard (0 pg/ml).

Standard	Add	Into
1000 pg/ml	200.0 μ l of the std.(5 ng/ml)	800.0 μ l of the <i>Standard/Sample Dilution Buffer</i>
500 pg/ml	500 μ l of the std.(1 ng/ml)	500.0 μ l of the <i>Standard/Sample Dilution Buffer</i>
250 pg/ml	500 μ l of the std.(500pg/ml)	500.0 μ l of the <i>Standard/Sample Dilution Buffer</i>
125 pg/ml	500 μ l of the std.(250 pg/ml)	500.0 μ l of the <i>Standard/Sample Dilution Buffer</i>
62.5 pg/ml	500 μ l of the std.(125 pg/ml)	500.0 μ l of the <i>Standard/Sample Dilution Buffer</i>
31.25 pg/ml	500 μ l of the std.(62.5 pg/ml)	500.0 μ l of the <i>Standard/Sample Dilution Buffer</i>
15.625 pg/ml	500 μ l of the std.(31.25 pg/ml)	500.0 μ l of the <i>Standard/Sample Dilution Buffer</i>
0 pg/ml	1.0 ml of the <i>Standard/Sample Dilution Buffer</i>	

2) Secondary Antibody

100X secondary antibody solution can be made by adding 150 μ l *Secondary antibody/Streptavidin HRP dilution buffer* in the vial.

1. Equilibrate to room temperature, mix gently.

2. Mix 20 µl *Secondary Antibody concentrated solution* (100X) + 1.98 ml *Secondary antibody/Streptavidin HRP dilution buffer*. (Sufficient for two 8-well strip, prepare more if necessary)

Label as “Working Secondary antibody Solution”.

3. Return the unused *Secondary Antibody concentrated solution* to the refrigerator.

3) Streptavidin HRP(X100)

1. Equilibrate to room temperature, mix gently.
2. Mix 20 µl *Streptavidin HRP concentrated solution* (100X) + 1.98 ml *Secondary antibody/Streptavidin HRP dilution buffer*. (Sufficient for two 8-well strip, prepare more if needed)

Label as “Working Streptavidin HRP Solution”.

3. Return the unused *Streptavidin HRP concentrated solution* to the refrigerator.

4) Washing buffer

1. Equilibrate to room temperature, mix to re-dissolve any precipitated salt.
2. Mix 0.5 volume *Wash buffer concentrate solution* (20X) + 9.5 volumes of deionized water. Label as “Working Washing Solution”.
3. Store both the concentrated and the Working Washing Solution in the refrigerator.

* Directions for washing

1. Fill the wells with 300 µl of “Working Washing Buffer”.

Let soak for 1 to 3 minutes and then all residual wash-liquid must be drained from the wells by aspiration (taking care not to scratch the inside of the well) or decantation, followed by forceful tapping of the plate on absorbent paper. Never insert absorbent paper directly into the wells.

If using an automated washer, the operating instructions for washing equipment should be carefully followed.

2. Incomplete washing will adversely affect the assay and renders false results.
3. It is recommended to use laboratory tape to hold plate strips to the plate frame while performing the plate washing to avoid strips coming free of the frame.

5) Sample preparation

Blood should be collected by venipuncture. For plasma samples, blood may be drawn into tubes containing sodium citrate or heparin, EDTA. The serum or plasma should be separated from the coagulated or packed cells by centrifugation. Samples may be shipped at room temperature and then stored refrigerated at 2-8°C if testing is to take place within one week after collection. If testing is to take place later than one week, samples should be stored at -20°C. Avoid repeated freeze/thawing.

9. Assay Procedure

- Allow all reagents to reach room temperature before use. Gently mix all liquid reagents prior to use.
 - All standards, controls and samples should be run in duplicate for confirmation of reproducibility.
 - A standard curve must be run with each assay.
 - If particulate matter is present in the analyte, centrifuge or filter prior to analysis.
 - Maintain a consistent order of components and reagents addition from well to well. This ensures equal incubation times for all wells.
- 1) Determine the number of 16-well strips needed for assay. Insert these in the flame(s) for current use (Re-bag extra strips and frame. Refrigerate for further use).
 - 2) For the standard curve, add 100 µl of the standard to the appropriate microtiter wells. Add 100 µl of the *Standard/Sample/secondary antibody Dilution Buffer* to zero wells.
 - 3) Serum and plasma require **at least 8 fold dilution** in the *Standard/Sample Dilution Buffer*. And add 100 µl of samples to each well.
 - 4) Cover the plate with the plate cover and incubate for 2 hours at 37°C.
 - 5) Thoroughly aspirate or decant the solution from the wells. Wash the wells 3 times (See “Directions for washing”).
 - 6) Pipette 100 µl of “Working Secondary Antibody Solution” into each well.
 - 7) Cover the plate with the plate cover and incubate for 1 hour at 37°C.
 - 8) Thoroughly aspirate or decant the solution from the wells. Wash the wells 3 times (See “Directions for washing”).
 - 9) Add 100 µl “Working Streptavidin HRP Solution” to each well.
 - 10) Cover the plate with the plate cover and incubate for 30 minutes at 37°C.
 - 11) Thoroughly aspirate or decant the solution from the wells. Wash the wells 3 times (See “Directions for washing”).
 - 12) Add 100 µl of *Substrate* to each well. The liquid in the wells should begin to turn blue.
 - 13) Incubate the plate at room temperature.
 - Do not cover the plate with aluminum foil, or color may develop. The incubation time for chromogen substrate is often determined by the microtiter plate reader used. O.D. values should be monitored and the substrate reaction stopped before O.D. of the positive wells exceeds the limits of the instrument. O.D. values at 450nm can only be read after the Stop Solution has been added to each well.
 - Because the *Substrate* is light sensitive, avoid the remained *Substrate* solution prolonged exposure to light.

- Typically, reaction is stopped 5~10 minutes after treatment of Substrate, but this time can be adjusted as the user desires.
- 14) Add 100 µl of *Stop Solution* to each well. The solution in the wells should change from blue to yellow.
 - 15) Read the absorbance of each well at 450nm. Read the plate within 20 minutes of adding the *Stop Solution*.
 - 16) Plot on graph paper the absorbance of the standard against the standard concentration (Optimally, the background absorbance can be subtracted from all data points, including standards, unknowns and controls, prior to plotting.). Draw a smooth curve through these points to construct the standard curve.
 - 17) Read the Rat MCP-1 concentrations for the unknown samples and controls from the standard curve plotted in step 18. Multiply value(s) obtained for the unknown sample by the dilution factor (Samples producing signals greater than that of the highest standard should be further diluted in the *Standard/Sample Dilution Buffer*).

10. Characteristics

1) Typical result


The standard curve below is for illustration only and **should not be used** to calculate results in your assay.

A standard curve must be run with each assay.

Standard Rat MCP-1 (pg/ml)	Optical Density (at 450nm)
0	0.091
15.625	0.120
31.25	0.154
62.5	0.216
125	0.368
250	0.679
500	1.190
1000	1.867

< Limitations >

- Do not extrapolate the standard curve beyond the 1000 pg/ml standard point.
- Other buffers and matrices have not been investigated.
- The rate of degradation of native Rat MCP-1 in various matrices has not been investigated.

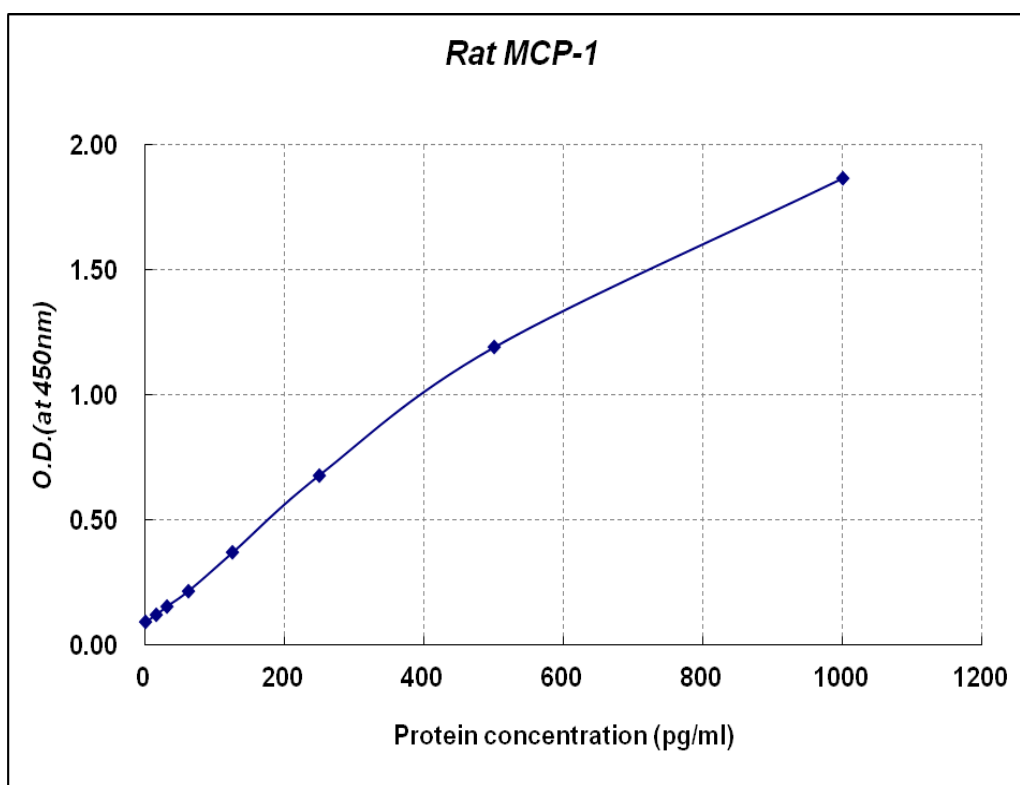

(TMB reaction incubate at room temperature for 5 min)

2) Sensitivity

The minimal detectable dose of Rat MCP-1 was calculated to be 8.221 pg/ml, by subtracting three standard deviations from the mean of 12 zero standard replicates (ELISA buffer, S0) and intersecting this value with the standard curve obtained in the same calculation.

<i>N</i>	<i>1</i>	<i>2</i>	<i>3</i>	<i>4</i>	<i>5</i>	<i>6</i>	<i>7</i>	<i>8</i>	<i>9</i>	<i>10</i>	<i>11</i>	<i>12</i>
ZERO	0.089	0.093	0.100	0.095	0.091	0.094	0.087	0.094	0.091	0.082	0.087	0.084

Average	SD	LLD	LLD mean(pg/ml)
0.091	0.005	0.106	8.221

3) Specificity

The following substances were tested and found to have no cross-reactivity: Human MCP-1, Mouse MCP-1.

4) Precision

① Within-Run (Intra-Assay)

(n=12)

Mean (pg/ml)	SD (pg/ml)	CV (%)
128.125	6.900	5.385
246.054	19.234	7.817
466.877	17.161	3.676
937.701	63.213	6.741

② Between-Run (Inter-Assay)

(n=12)

Mean (pg/ml)	SD (pg/ml)	CV (%)
127.397	12.241	9.608
246.840	12.746	5.164
522.130	22.483	4.306
977.486	17.167	1.756

5) Recovery

Recovery on addition is 94.261~111.317% (mean 102.483%)

Added Analyte (pg/ml)	Serum(1/64)+added analyte (450nm)	Serum(1/64)(450nm) +added analyte(450nm)	Recovery (%)
126.569	293.583	276.735	94.261
247.808	414.822	426.029	102.702
500.989	668.003	679.046	101.653
999.866	1166.88	1298.940	111.317

11. Troubleshooting

Problem	Possible Cause	Solution
High signal and background in all wells	<ul style="list-style-type: none"> • Insufficient washing 	<ul style="list-style-type: none"> • Increase number of washes • Increase time of soaking between in wash
	<ul style="list-style-type: none"> • Too much Streptavidin-HRP 	<ul style="list-style-type: none"> • Check dilution, titration
	<ul style="list-style-type: none"> • Incubation time too long 	<ul style="list-style-type: none"> • Reduce incubation time
	<ul style="list-style-type: none"> • Development time too long 	<ul style="list-style-type: none"> • Decrease the incubation time before the stop solution is added
No signal	<ul style="list-style-type: none"> • Reagent added in incorrect order, or incorrectly prepared 	<ul style="list-style-type: none"> • Review protocol
	<ul style="list-style-type: none"> • Standard has gone bad (If there is a signal in the sample wells) 	<ul style="list-style-type: none"> • Check the condition of stored standard
	<ul style="list-style-type: none"> • Assay was conducted from an incorrect starting point 	<ul style="list-style-type: none"> • Reagents allows to come to 20~30°C before performing assay
Too much signal – whole plate turned uniformly blue	<ul style="list-style-type: none"> • Insufficient washing –unbound SAV-HRP remaining 	<ul style="list-style-type: none"> • Increase number of washes carefully
	<ul style="list-style-type: none"> • Too much Streptavidin -HRP 	<ul style="list-style-type: none"> • Check dilution
	<ul style="list-style-type: none"> • Plate sealer or reservoir reused, resulting in presence of residual Streptavidin -HRP 	<ul style="list-style-type: none"> • Use fresh plate sealer and reagent reservoir for each step
Standard curve achieved but poor discrimination between point	<ul style="list-style-type: none"> • Plate not developed long enough 	<ul style="list-style-type: none"> • Increase substrate solution incubation time
	<ul style="list-style-type: none"> • Improper calculation of standard curve dilution 	<ul style="list-style-type: none"> • Check dilution, make new standard curve
No signal when a signal is expected, but standard curve looks fine	<ul style="list-style-type: none"> • Sample matrix is masking detection 	<ul style="list-style-type: none"> • More diluted sample recommended
Samples are reading too high, but standard curve is fine	<ul style="list-style-type: none"> • Samples contain protein levels above assay range 	<ul style="list-style-type: none"> • Dilute samples and run again
Edge effect	<ul style="list-style-type: none"> • Uneven temperature around work surface 	<ul style="list-style-type: none"> • Avoid incubating plate in areas where environmental conditions vary • Use plate sealer

12. Reference

- 1) Carr, M. W.; Roth, S. J.; Luther, E.; Rose, S. S.; Springer, T. A. (1994). "Monocyte chemoattractant protein 1 acts as a T-lymphocyte chemoattractant". *Proceedings of the National Academy of Sciences of the United States of America* **91** (9): 3652–3656.
- 2) Xu, L. L.; Warren, M. K.; Rose, W. L.; Gong, W.; Wang, J. M. (1996). "Human recombinant monocyte chemotactic protein and other C-C chemokines bind and induce directional migration of dendritic cells in vitro". *Journal of leukocyte biology* **60** (3): 365–371.
- 3) Conti, P.; Boucher, W.; Letourneau, R.; Feliciani, C.; Reale, M.; Barbacane, R. C.; Vlagopoulos, P.; Bruneau, G.; Thibault, J.; Theoharides, T. C. (1995). "Monocyte chemotactic protein-1 provokes mast cell aggregation and 3H5HT release". *Immunology* **86** (3): 434–440.
- 4) Bischoff, S. C.; Krieger, M.; Brunner, T.; Dahinden, C. A. (1992). "Monocyte chemotactic protein 1 is a potent activator of human basophils". *The Journal of experimental medicine* **175** (5): 1271–1275.
- 5) Kim, M. S.; Day, C. J.; Morrison, N. A. (2005). "MCP-1 is Induced by Receptor Activator of Nuclear Factor- κ B Ligand, Promotes Human Osteoclast Fusion, and Rescues Granulocyte Macrophage Colony-stimulating Factor Suppression of Osteoclast Formation". *Journal of Biological Chemistry* **280** (16): 16163–16169.
- 6) Banisadr, G.; Gosselin, R. D.; Mechighel, P.; Kitabgi, P.; Rostène, W.; Parsadaniantz, S. P. M. L. (2005). "Highly regionalized neuronal expression of monocyte chemoattractant protein-1 (MCP-1/CCL2) in rat brain: Evidence for its colocalization with neurotransmitters and neuropeptides". *The Journal of Comparative Neurology* **489** (3): 275–292.

◆ Ordering Information

For orders, please contact :

Immuno-Biological Laboratories, Inc. (IBL-America)

Address: 8201 Central Ave NE, Suite P, Minneapolis, MN 55432

Toll Free: (888) 523-1246

Fax: (763) 780-2988

E-mail: info@ibl-america.com

Website: www.ibl-america.com

For technical advice, please contact:

E-mail : info@ibl-america.com

Website : www.ibl-america.com