


# IGF-I RIA

Radioimmunoassay for Quantitative Determination of

## Insulin-like Growth Factor I (IGF-I) (IGFBP-blocked)

For Research Use Only.  
Not for use in diagnostic procedures.

+2°C  +8°C



for 200 Tubes



**REF R21**



Distributed By:

**IBL-America, Inc.**


8201 Central Ave NE, Suite P  
Minneapolis, MN 55432, USA

[info@ibl-america.com](mailto:info@ibl-america.com)

(888) 523 1246



Gesellschaft für Forschung und Herstellung von Diagnostika GmbH

 Aspenhastr. 25 • D-72770 Reutlingen / Germany  
Phone: + 49 - (0) 7121 51484-0 • Fax: + 49 - (0) 7121 51484-10  
E-mail: [contact@mediagnost.de](mailto:contact@mediagnost.de) • <http://www.mediagnost.de>

## Symbols DIN EN ISO 15223-1



Expiry date



Consider instructions for use



Lot-Batch Number



Manufactured by



Catalogue Number



Store at between



Contains sufficient for x tests



Radioactive

For Research Use Only

# Table of Contents

1	INTENDED USE .....	4
2	INTRODUCTION .....	4
3	PRINCIPLE.....	5
4	WARNINGS AND PRECAUTIONS .....	6
5	SAMPLES.....	7
6	MATERIALS.....	8
7	TECHNICAL NOTES.....	9
8	ASSAY PROCEDURE.....	10
9	CALCULATION OF RESULTS .....	11
10	LIMITATIONS OF PROCEDURE.....	12
11	EXEMPLARY VALUES .....	12
12	PERFORMANCE CHARATERISTICS.....	14
13	ASSAY COMPARISON .....	16
14	REFERENCES.....	17
15	ASSAY PROCEDURE .....	20

For Research Use Only

## Information for Use

IGF-I RIA, R21	200 Determinations
Principle of the test	Non - extractive radioimmunoassay
Duration (incubation period)	2 days + 1.5 h
Tracer	Iodinated recombinant IGF-I, < 55 kBq
Antibodies	specific, high-affinity polyclonal antiserum
Cross reactivity with IGF-II	< 0.103 %
Buffer	Ready to use
Reference material	International Standard WHO/NIBSC 02/254
Calibrator	8 single calibrators: 0 – 10 ng/mL, recombinant IGF-I
Assay Range	0.064 – 1010 ng/mL
Control	2 control sera, freeze-dried - RiliBäK conform
Sample	human serum / plasma
Required sample volume	10 µL
Sample dilution	1:101
Analytical sensitivity	∅ 0.064 ng/mL
Intra- / Interassay Variance	∅ 4.76 / 5.06 %
Half Maximal displacement	at < 3.5 ng/mL

### 1 INTENDED USE

This radioimmunoassay kit is intended to be used for research only. It quantifies human IGF-I in serum, plasma, or other human biological fluids (e.g. follicular fluid, seminal plasma).

### 2 INTRODUCTION

Insulin-like growth factors (IGF) I and II play a pivotal role in regulating the proliferation, differentiation and specific functions of many cell types (1-3). IGF-I is identical with Somatomedin C (Sm-C) (4) and has a molecular weight of 7649 daltons (5). Its major regulators are growth hormone (GH) and nutrition (6), although its production in specific tissues is affected by a multitude of tropic hormones and other peptide growth factors. In contrast to many other peptide hormones, IGFs are avidly bound to specific binding proteins (IGFBP). The seven classes of IGFBPs which are known at present (7,8,22) either bind IGF-I and IGF-II with similar affinities or show a preference for IGF-II (9,10).

A major problem of IGF-I measurement results from the interference of IGFBPs in the assay. Direct determinations in untreated serum samples (11) give false values because of the extremely slow dissociation of the IGF-I/IGFBP-3 complexes during the assay incubation. Depending on the ratio IGF-I to IGFBP the following errors may occur:

-in samples with low IGF-I concentration, IGFBP-complexation will take place predominantly with the IGF-I tracer, thus leading to false-high results in a competitive RIA. Effect: Overestimation of low IGF-I levels.


-in samples with high IGF-I concentration, unmarked IGF-I from the sample will be predominantly complexed by IGFBPs and therefore withdrawn from measurement. Effect: Underestimation of high IGF-I levels.

Therefore, various techniques were applied to physically separate IGF-I from its binding proteins before measurement, including (a) size exclusion chromatography under acidic conditions, (b) solid-phase extraction and (c) acid-ethanol extraction (2,12,13). These techniques, however, are either inconvenient or time-consuming or give incomplete and not-reproducible recoveries. The most widely used method is the acid-ethanol extraction (13,14) with a recovery of only 70-80 % of IGFBP-bound IGF-I as a result of co-precipitation. The absolute results of such an extraction are therefore false low (15). The extraction removes the IGFBPs only insufficiently and leads to reduction in sensitivity of the assay due to pre-

dilution of the samples by the extraction procedure. Furthermore, the remaining IGFBP may still interfere in the assay. In addition, the acid-ethanol extraction is ineffective in specimens other than serum or plasma (e.g. cell culture media), in which determination of IGF-I is already difficult enough due to the fact that IGFBPs are frequently present at large excess. To avoid these difficulties, an uncomplicated assay was developed, in which special sample preparation is not required before measurement.

### 3 PRINCIPLE

In order to dissociate IGF-I from the IGFBPs, the samples must be diluted in an acidic buffer (Figure 1). The diluted samples are then pipetted into the assay tubes. The IGF-I antiserum containing an excess of IGF-II is dissolved in a buffer, which is able to neutralize the acidic samples.

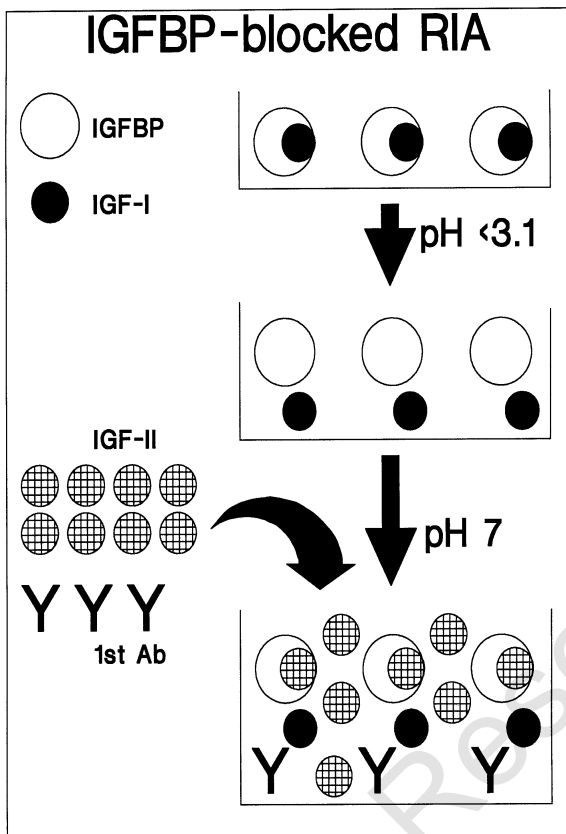

After the IGF-I antibody solution has neutralized the samples, the excess IGF-II occupies the IGF-binding sites of the binding proteins, thus allowing the measurement of free IGF-I. With this method, the IGFBPs are not removed, but their function and therefore their interference in the assay is neutralized.

Due to the extremely low cross-reactivity of the IGF-I antibody with IGF-II, excess IGF-II does not disturb the interaction of the first antibody with IGF-I or IGF-I tracer. The assay is then continued like a conventional RIA using a second antibody for the separation of bound and free tracer.

The colour of the solutions makes possible for every tube a control of the respective performance step. This enables you to check your pipette plan, if necessary. Dilution and acidification buffer (including the reconstituted calibrators and diluted samples too) are coloured in green through addition of a pH indicator dye. After addition of the uncoloured IGF-I antibody solution, the now neutralized solutions turn blue. Finally, addition of the red coloured tracer solution turns the entire incubation colour violet.

Figure 1 Principle of the IGFBP-blocked IGF-I RIA

## 4 WARNINGS AND PRECAUTIONS

1. For Research Use Only. Not for use in diagnostic procedures.
2. For professional use only.
3. The acquisition, possession and use of the kit are subject to the regulations of the national nuclear regulatory authorities.
4. Before starting the assay, read the instructions completely and carefully. Use the valid version of the package insert provided with the kit. Be sure that everything is understood.
5. Before use, all kit components should be brought to room temperature at 20 - 25 °C (68 - 77 °F). Precipitates in buffers should be dissolved before use by thorough mixing and warming.
6. Do not mix reagents of different lots. Do not use expired reagents.
7. **Caution:** This kit contains material of human and/or animal origin. Source human serum for the Control Serum provided in this kit was tested by recommended methods and found non-reactive for Hepatitis-B surface antigen (HBsAg), Hepatitis C virus (HCV), and Human Immunodeficiency Virus 1 and 2 (HIV) antibody. No known test methods can offer total assurance of the absence of infectious agents; therefore all components and specimens should be treated as potentially infectious.
8. Reagents contain Sodium-Azide (0.02%) as preservative, however highly diluted. Safety Data Sheet available on request.
9. Do not use obvious damaged or microbial contaminated or spilled material.

10. Radioactivity - Radioactive material may be received, acquired, possessed, and used only by physicians, veterinarians in the practice of veterinary medicine, clinical laboratories, or hospitals and only for in vitro clinical or laboratory tests not involving internal or external administration of the material, or the radiation there from, to human beings or animals. Its receipt, acquisition, possession, use, and transfer are subject to the regulations and a general license of the state commissioner of health, the Nuclear Regulatory Commission, or a state with which the Nuclear Regulatory Commission has entered into an agreement for the exercise of regulatory authority. Before ordering or using radioactive materials, it is necessary to take the appropriate actions to ensure compliance with national regulations governing their use. Local rules in each establishment, which define actions and behavior in the radioactivity working areas, should also be adhered to. The advice given here does not replace any local rules, instructions or training in the establishment, or advice from the radiation protection advisers. It is important to follow the code of good laboratory practice in addition to the specific precautions relating to the radionuclide I-125 used.

Iodine-125 has a radioactive half-life  $T_{1/2}$  of 60 days and emits 35.5 keV gamma radiation, 27 – 32 keV x-rays and no beta radiation. Shielding is effectively done by lead, first half value layer is 0.02 mm lead, reduction to 10 % is made by 0.2 mm.

To reduce the radiation dose time spent handling radioactivity should be minimized (plan ahead), and distance from source of radiation should be maximized (doubling the distance from the source quarters the radiation dose).

Formation of aerosols, e.g. by improper opening and mixing of vials or pipetting of solutions which may cause minute droplets of radioactivity become airborne, is a hazard and should be avoided. Solutions containing iodine should not be made acidic, because this might lead to the formation of volatile elemental iodine.

As some iodo-compounds can penetrate rubber gloves, it is advisable to wear two pairs or polyethylene gloves over rubber.

For cleaning of contaminated areas or equipment, the Iodine-125 should be rendered chemically stable by using alkaline sodium thiosulphate solution together with paper or cellulose tissue.

### **General First Aid Procedures:**

*Skin contact:* Wash affected area thoroughly with water at least 15 minutes. Discard contaminated cloths and shoes. See a physician.

*Eye contact:* In case of contact with eyes, rinse immediately with plenty of water at least 15 minutes. In order to assure an effectual rinsing spread the eyelids. See a physician.

*Ingestion:* If swallowed, wash out mouth thoroughly with water, provided that the person is conscious. Immediately see a physician.

The handling of radioactive and potentially infectious material must comply with the following guidelines:

The material should be stored and used in a special designated area.

Do not eat, drink or smoke in these areas.

Never pipette the materials with the mouth.

Avoid direct contact with these materials by wearing laboratory coats and disposable gloves.

Spilled material must be wiped off immediately. Clean contaminated areas and equipment with a suitable detergent.

Unused radioactive material and radioactive waste should be disposed according to the recommendations of the national regulatory authorities.

## 5 SAMPLES

### 5.1 Sample Type

Serum and Plasma

Serum and Heparin/EDTA Plasma yield comparable values.

The IGF-I levels are reduced in citrate plasma samples, because of the relatively high amount of anticoagulant.

Mediagnost R21 can be also used for measurement of matrices with low concentrations of IGF-I like saliva, cerebrospinal fluid, urine, breast milk and cell culture supernatant. Matrices other than serum and plasma cannot be diluted but acidified by adding Acidification Buffer **AB**.

### 5.2 Specimen collections

Use standard venipuncture for the blood sampling. Haemolytic reactions are to be avoided. Blood samples may be taken at any time of the day. Whole blood should be processed within a few hours and stored frozen at -20 °C (-4 °F) until measurement.

### 5.3 Required sample volume

10 µL

### 5.4 Sample stability

In firmly closable sample vials

- Storage at **20 - 25 °C** (68 - 77 °F): max. 6 days
- Storage at **-20 °C** (-4 °F): min. 2 years
- Freezer /-thaw cycles max. 3

The storage of samples over a period of 2 years at **-20 °C** (-4 °F), showed no influence on the measurement. Freezing and thawing of samples should be minimized. 3 Freezing-/ Thawing showed no effect on samples.

### 5.5 Interference

Either triglycerides, bilirubin nor hemoglobin exert any influence up to concentrations of 100 g/L, 200 mg/L, 5 g/L respectively on the measurement of IGF-I in human serum. Rec.IGFBP-3 don't interfere with IGF-I measurement up to the concentration of 12 mg/L in Dilution Buffer **DB**.


### 5.6 Sample dilution

- **Dilution: 1:101** with Dilution Buffer **DB**  
**Example:** Add **10 µL** Sample to **1 mL Dilution Buffer DB** (101 dilution factor).
- The **serum and plasma samples** must be diluted at least **1:20 in Dilution Buffer DB**.
- Matrices **other than serum and plasma** must be acidified by adding **Acidification Buffer AB** (1/10th of the sample volume).  
**Example:** Add **20 µL Acidification Buffer AB** to **200 µL** sample (dilution factor: 1.1).

## 6 MATERIALS

### 6.1 Reagents provided

The reagents listed below are sufficient for 200 tubes including the calibrator curve.

<b>*AB</b>	<b>Acidification Buffer</b> , ready for use, coloured	<b>1 x 12.5 mL</b>
<b>DB</b>	<b>Dilution Buffer</b> , ready for use, coloured	<b>2 x 125 mL</b>
<b>A</b>	<b>Assay Buffer</b> ready for use	<b>2 x 30 mL</b>
<b>B</b>	<b>1st Antibody</b> , lyophilized (anti-hIGF-I) contains rabbit IgG and rec. hIGF-II	<b>2 x 11 mL</b>
<b>C</b>	<b>Tracer: <sup>125</sup>I-IGF-I</b> , lyophilized, < 1.5 µCi or < 55 kBq - red coloured	<b>2 x 11 mL</b>
<b>D</b>	<b>Non-Specific Binding (NSB)</b> , lyophilized, Rabbit immunoglobulin	<b>1 x 500 µL</b>
<b>E - L</b>	<b>Calibrators</b> , lyophilized, (rec. Human IGF-I) Concentrations given on vial-labels in ng/mL	<b>8 x 500 µL</b>
<b>M</b>	<b>Control High</b> , lyophilized (human serum): Concentration see certificate - lyophilized	<b>1 x 100 µL</b>
<b>N</b>	<b>Control Low</b> , lyophilized (human serum): Concentration see certificate - lyophilized	<b>1 x 100 µL</b>
<b>O</b>	<b>2nd Antibody</b> , lyophilized (anti-rabbit immunoglobulin)	<b>2 x 1 mL</b>
<b>P</b>	<b>Precipitation Reagent</b> ready for use after adding <b>O</b>	<b>2 x 55 mL</b>
	<b>Instructions for use</b>	<b>1 x</b>
	<b>Quality Certificate</b>	<b>1 x</b>

### 6.2 Reagents required, but not provided

- Cold demineralised water or distilled water (Aqua destillata) (**A. dest.**)
- Pipettes: 10 mL, 1 mL, 500 µL, 100 µL, 10 µL;  
100 µL, 500 µL and 1 mL repeating pipettes are recommended.
- Disposable polystyrene or polypropylene tubes. Conical tubes are highly recommended because of the small immune precipitates. The use of round-bottom tubes may cause formation of insufficiently compact pellets.
- Vortex mixer
- Centrifuge
- Device for aspiration of liquid supernatant
- Gamma counter

\*The IGF-I measurement in other matrices than serum or plasma is possible. The reagent: **Acidification Buffer AB** is included in the kit for these applications.



## 7 TECHNICAL NOTES

### 7.1 Storage Conditions

Store the kit at **2 - 8 °C (35.6 - 46.4 °F)** after receipt until its expiry date. The lyophilized reagents should be stored at **-20 °C (-4 °F)** after reconstitution. Avoid repeated thawing and freezing. The shelf-life of the **reagents after opening** is in accordance with the Tracer **C** shelf life.

### 7.2 Reagent Preparation

Ensure that lyophilized materials are completely dissolved on reconstitution. It is recommended to touch the tubes with lyophilized material once on a solid base before first opening in order to accumulate the material at the bottom of the tubes. It is recommended to keep the reconstituted reagents at **20 - 25 °C (68 - 77 °F)** for half an hour and then to mix them vigorously with a Vortex mixer. This is important in particular for the Controls **M** and **N**.

- B** Reconstitute with **11 mL** Assay Buffer **A**.
- C** Reconstitute with **11 mL** Assay Buffer **A**.
- D** Reconstitute with **500 µL** Assay Buffer **A**.
- E - L** Reconstitute with **500 µL** Dilution Buffer **DB**.
- M** Reconstitute with **100 µL A. dest.** Further dilution according to sample dilution with Dilution Buffer **DB** (e.g. 1:101).
- N** Reconstitute with **100 µL A. dest.** Further dilution according to sample dilution with Dilution Buffer **DB** (e.g. 1:101).
- O** Reconstitute with **1 mL** Assay Buffer **A**. Transfer dissolved material to Reagent **P** immediately before use. For 100 tubes add 1 vial reagent **O** (reconstituted in **1 mL A**) to 1 bottle of reagent **P** (**55 mL**) or any volumes in the same ratio (1:56) for less tubes. The assay is unaffected by the possible occurrence of turbidity in the final reagent.

## 8 ASSAY PROCEDURE

### Flow Chart of Assay Protocol:

Nr. of tubes	Contents of tube	DB E-L M,N Samples	D	B	C	P
1, 2	Total Counts	---	---	---	100	---
3, 4	NSB	100 <b>DB</b>	100	---	100	500
5, 6	B <sub>0</sub>	100 <b>E</b>	---	100	100	500
7 - 20	Calibrators	100 <b>F-L</b>	---	100	100	500
21, 22	High Control	100 <b>M</b>	---	100	100	500
23, 24	Low Control	100 <b>N</b>	---	100	100	500
25, 26	Sample 1	100	---	100	100	500
27, 28	Sample 2	100	---	100	100	500
etc.						
<b>Colour after addition:</b>		Green	Blue		Violet	

**Note:** All volumes are given as  $\mu\text{L}$ .

Samples (calibrators, controls and samples) should be assayed in duplicate. For optimal results, accurate pipetting and adherence to the test-protocol are recommended. Before use, all kit components should be brought to room temperature at **20 - 25 °C (68 - 77 °F)**, except reagent **P**.

- 1) Labelling of the assay tubes (duplicates) should be done in the following order: 1 and 2 **total counts**, 3 and 4 **NSB**, 5 and 6 **zero calibrator (B<sub>0</sub>)**, 7 to 20 **calibrators**, 21 to 24 controls, 25 to 100 **samples**.
- 2) Add **100  $\mu\text{L}$**  of Dilution Buffer **DB** to tubes 3 and 4.
- 3) Add **100  $\mu\text{L}$**  of reagents **E - L (calibrators)** to tubes 5 to 20, (**zero calibrator (E)** to tubes 5 and 6, **calibrator F** (0.156 ng/mL) to tubes 7 and 8, etc).
- 4) Add **100  $\mu\text{L}$**  of diluted reagent **M (high control)** to tubes 21 and 22 and **100  $\mu\text{L}$**  of diluted reagent **N (low control)** to tubes 23 and 24.
- 5) Add **100  $\mu\text{L}$**  of diluted (or only acidified) **samples** to tubes 25 and 26, etc. - All solutions appear **green!**
- 6) Add **100  $\mu\text{L}$**  reagent **D (NSB)** to tubes 3 and 4. -The solutions turn **blue**.
- 7) Add **100  $\mu\text{L}$**  reagent **B (1st Antibody)** beginning with tube 5. -The solutions turn **blue!**
- 8) Add **100  $\mu\text{L}$**  reagent **C (tracer)** to all tubes. - All solutions turn **violet!**
- 9) Remove tubes 1 and 2 (**total counts**) or mark or seal with a stopper.
- 10) Mix tubes with a vortex mixer.
- 11) Incubate tubes at **2 - 8 °C (35.6 - 46.4 °F)** for **2 days**. Incubation for a longer period (e.g. **over the weekend**) has no negative effect on the results.
- 12) Add **500  $\mu\text{L}$**  reagent **P** (after addition of reagent **O**), beginning with tube 3. The reagent should be cold **2 - 8 °C (35.6 - 46.4 °F)**.
- 13) Mix tubes with a vortex mixer.
- 14) Incubate tubes at **2 - 8 °C (35.6 - 46.4 °F)** for **1 hour**.
- 15) Add **1 mL ice-cold distilled water**.
- 16) Centrifuge all tubes except tubes 1 and 2 at least at **3000 x g** for **30 min** at a temperature of **2 - 8 °C (35.6 - 46.4 °F)**.
- 17) Aspirate the supernatant (except tubes 1 and 2 !). The remaining supernatant should be about 2 mm above the precipitate. Take care that the precipitate remains intact. Depending on local conditions and procedures, the supernatant may also be decanted instead of aspirated.
- 18) Count the activity of **all** tubes (including tubes 1 and 2) for **1 to 3 min**.

## 9 CALCULATION OF RESULTS

### 9.1 Establishing of the Calibrator Curve

The calibrators provided contain the following concentrations of IGF-I:

Calibrator	E	F	G	H	I	J	K	L
ng/mL	0.0	0.156	0.313	0.625	1.25	2.5	5.0	10

1. Calculate the average counts of each pair of tubes.
2. Subtract the average counts of NSB tubes (3 and 4) from the mean counts of the calibrators, controls and samples. This gives the corrected values for B.
3. The corrected value from the zero calibrator E (tubes 5 and 6) is  $B_0$ .
4. Calculate the percent bound (% B/ $B_0$ ) by dividing the corrected B-values by  $B_0$ :  $B/B_0 \times 100\%$ .
5. Plot % B/ $B_0$  versus the calibrator concentrations on either semi-logarithmic or logit-log paper. For convenience, it is recommended to use computer assisted data reduction programs.
6. For quality control calculate NSB in %: average counts of tubes 3 and 4 divided by the average counts of tubes 1 and 2 (Total Count, TC) times 100%. It should be < 5% (%NSB/TC < 5).

Calculate the percent bound of the zero calibrator E: average counts of tubes 5 and 6 minus average counts of NSB divided by TC times 100%. It should be > 25% (% $B_0$ /TC > 25).

Example:	
<b>unspecific</b> Binding in [%]:	<b>specific</b> Binding in [%]:
NSB / Total activity TC x 100 = 510 / 23435 x 100 = 2.2%	$B_0$ / Total activity TC x 100 = (10984 – 510) / 23435 x 100 = 44.7%

	Example	Target Value
Unspecific Binding: %NSB/TC	2.2	< 5.0
Specific Binding % $B_0$ /TC	44.7	> 25

### 9.2 Example of Typical Calibrator Curve

The following data is for demonstration only and cannot be used in place of data generation at the time of assay.

	E ( $B_0$ )	F	G	H	I	J	K	L	TC	NSB
ng/mL	0.0	0.156	0.313	0.625	1.25	2.5	5.0	10	-	-
cpm	10984	10369	9689	8720	7270	5461	3709	2423	23435	510

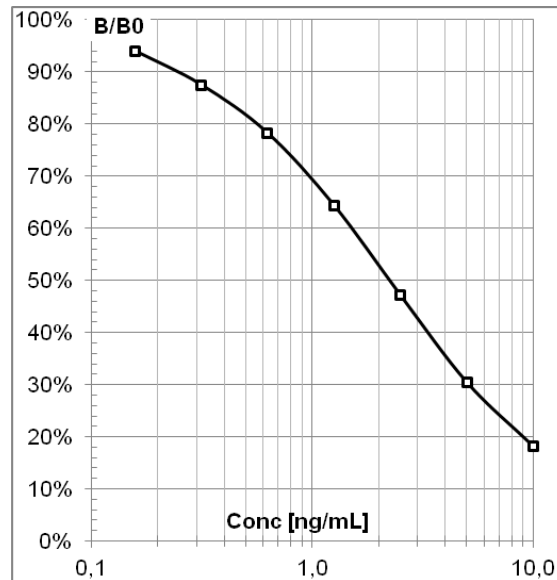


Figure 2 Exemplary Calibrator Curve.

### 9.3 Evaluation of sample concentration

Read the concentration value (abscissa) corresponding to the % B/B0 of the sample as in the example given below:

Average counts of <b>NSB (D):</b>	<b>510 cpm</b>
Average counts of zero calibrator <b>E (B0):</b>	<b>10984 cpm</b>
Average counts of sample:	<b>6311 cpm</b>
<b>%B/B0 = (sample counts- NSB) / (B0 - NSB) x 100</b>	
= (6311 - 510) / (10984 - 510) x 100	
= 0.5539 x 100	
= <b>55.39 %</b>	

For a 55.39 %-value on the y-axis (ordinate) a value of 1.81 ng/mL on the x-axis (abscissa) was obtained. Multiply the concentration value determined graphically or by the aid of a computer program with the dilution factor (e.g.: 101).

Example: 1.81 x 101 = 183 ng/mL

In order to express the results as nmol/L the values given as ng/mL should be divided by 7.649 (molecular weight of IGF-I in kilo dalton).

Example: 183 ng/mL: 7.649 = 23.9 nmol/L

### 9.4 Concentration of control samples

The IGF-I concentration of Controls **M&N** should be within the ranges given on the certificate.

## 10 LIMITATIONS OF PROCEDURE

Generally, immunological assays are sensible to heterophilic antibodies and rheumatoid factors in the sample. Their influence is reduced by the assay design, but cannot be excluded completely.

## 11 EXEMPLARY VALUES

IGF-I levels are highly age-dependent in children, less so in adults until the age of about 60. The exemplary ranges in various age groups, which are log-normally distributed, are given in Table 2 by percentiles.

Between 8 and 19 years of age, values are given for boys and girls separately, because the pubertal peak usually occurs approximately 2 years earlier in girls.

**Table 1** Exemplary range of serum IGF-I levels given in ng/mL at different pubertal stages according to Tanner. Because no significant difference between boys and girls is observed, both sexes are combined. Only children and adolescents between 7 and 17 years of age are included.

Percentile				
Pubertal Stage	0.1th	5th	50th	95th
1	61	105	186	330
2	85	156	298	568
3	113	196	352	631
4	171	268	431	693
5	165	263	431	706

**Table 2** Serum levels of IGF-I in healthy subjects at various ages. Individuals between 8 and 19 years of age were classified according to gender, as the pubertal peak occurs almost 2 years earlier in girls than in boys.

Percentile														
Age	0.1	1	5	10	20	30	40	50	60	70	80	90	95	99
0-2 y.	13	20	28	34	43	50	58	66	75	87	102	128	156	220
2-4 y.	20	29	40	48	59	68	77	87	98	111	129	159	189	260
4-6 y.	26	36	50	59	73	85	96	108	122	138	160	196	233	320
6-7 y.	34	46	62	72	87	99	111	124	138	155	176	212	248	332
7-8 y.	45	60	78	90	107	121	134	148	163	181	205	243	281	364
8-9 y. boys	54	71	90	102	119	133	146	160	175	192	214	250	284	362
girls	55	75	99	115	137	156	174	193	214	239	271	324	376	496
9-10 y. boys	63	82	102	115	133	148	162	176	191	209	232	269	304	379
girls	68	89	114	130	152	170	187	205	224	247	276	323	369	469
10-11 y. boys	77	96	117	130	148	162	176	189	203	220	241	274	305	370
girls	81	106	134	153	178	199	219	239	261	287	321	374	426	539
11-12 y. boys	85	106	129	144	163	179	194	209	225	244	267	304	339	413
girls	91	123	160	185	220	248	276	305	337	374	424	503	581	758
12-13 y. boys	88	112	141	159	184	204	223	243	264	289	321	371	419	525
girls	116	155	201	231	274	309	342	377	415	460	519	614	707	914
13-14 y. boys	111	143	179	203	235	261	286	311	339	371	412	477	540	677
girls	163	207	256	287	329	364	395	428	463	504	556	637	716	884
14-15 y. boys	140	182	229	260	303	337	370	404	441	484	539	625	691	896
girls	193	236	284	314	353	385	414	443	474	510	556	628	713	832
15-16 y. boys	176	221	269	299	340	372	402	433	466	504	552	626	697	849
girls	187	231	279	309	350	382	412	442	474	512	559	632	700	845
16-17 y. boys	178	221	267	296	335	366	395	424	455	491	537	607	673	814
girls	183	225	270	298	336	366	394	422	452	486	530	597	660	792
17-18 y. boys	173	207	243	265	294	317	337	358	380	405	436	484	527	618
girls	176	210	246	268	297	320	341	362	384	409	441	488	533	624
18-19 y. boys	167	201	235	256	285	307	327	347	368	393	423	469	512	600
girls	167	199	233	254	281	302	322	341	362	385	414	458	499	583
19-20 y.	158	189	220	240	265	285	304	322	341	363	391	433	471	550
20-30 y.	72	92	115	130	150	167	182	198	215	235	261	302	340	425
30-40 y.	68	87	109	123	142	158	173	188	204	223	248	287	324	404
40-50 y.	64	82	103	116	135	150	164	178	194	212	235	272	310	385
50-60 y.	60	77	97	110	127	142	155	169	184	201	224	260	292	369
60-70 y.	55	72	91	103	120	134	147	161	176	193	215	251	282	362
70-80 y.	25	35	47	55	67	78	88	98	110	124	142	173	207	276
>80 y.	21	30	40	47	58	67	76	85	95	108	125	153	184	245

Serum concentrations are given in ng/mL.

Determined with IGFBP-blocked IGF-I RIA without extraction step (Blum and Breier 1994) (27).

Exemplary values have been evaluated by Prof. Blum by a radioimmunoassay identically composed to Mediagnost R21. Thus, these age and sex specific exemplary values can be applied to all Mediagnost IGF-I assays.

## 12 PERFORMANCE CHARACTERISTICS

### 12.1 Sensitivity

Sensitivity was assessed by measuring the  $B_0$  in 16-fold determination and calculating the theoretical concentration of the CPM of  $B_0$  (Mean Value - 2SD). The analytical sensitivity of the Mediagnost IGF-RIA is calculated to 0.064 µg/L (range: 0.02-0.109).

### 12.2 Specificity

The following materials have been evaluated for cross reactivity. 200 ng/mL solutions of each substance have been analysed in this Radioimmunoassay. No significant cross reactivity of the tested substances was detected (see table 3).

**Table 3** Cross reactivity of IGF-I related proteins

	IGF-II	Insulin	Proinsulin	C-Peptide
Reactivity [%]	0.103	0.005	0.012	0.019

### 12.3 Precision Data

#### Intra-Assay Variance

Six samples have been measured two to four times in the same assay. The results are shown in Table 4. The measured coefficient of variation (CV) is 4.76% on average (Range: 1.0 -16.1%).

**Table 4** Intra-Assay Variation was measured in independent test with different lots. Each sample was measured twice or four times within each assay and the %CV was calculated for each sample and each test.

%CV	Test 1	Test 2	Test 3	Test 4
Sample 1	1.8	1.9	3.4	4
Sample 2	3.4	11.4	6.4	16.1
Sample 3	4.6	5.8	2.8	6.3
Sample 4	3.3	2.0	2.8	4.7
Sample 5	3.9	6.2	1.0	7.3
Sample 6	2.7	3.2	2.9	6.3
Mean [%]	3.28	5.08	3.22	7.45

#### Inter-Assay Variance

Serum samples were measured in independent assays. On average the coefficient of variation was 5.06% (Range 4.46 – 6.00%). Exemplary results are shown in table 5.

**Table 5** Inter-Assay Variation measured as %CV of n-fold measured IGF-I concentration of different human serum in different kit lots within 18 months.

	Sample 1	Sample 2	Sample 3	Sample 4	Sample 5	Sample 6	Sample 7	Sample 8	Sample 9
Mean [µg/L]	300	263	172	200	298	151	428	309	196
SD [µg/L]	13.40	12.82	8.62	9.54	15.81	9.09	22.05	16.12	9.32
%CV	<b>4.46</b>	<b>4.87</b>	<b>5.01</b>	<b>4.77</b>	<b>5.30</b>	<b>6.00</b>	<b>5.16</b>	<b>5.22</b>	<b>4.75</b>
n	62	49	43	60	58	62	62	53	58

## Lot-to-Lot Variability

Several samples have been tested several times in different lots. In the below table the results of five serum samples are summarized.

**Table 6** Lot-to-Lot variability of IGF-I measurements. Exemplary results are shown for 5 serum samples measured repeatedly over a period of five years in 9 different lots.

	Sample 1	Sample 2	Sample 3	Sample 4	Sample 5
Mean	209.98	63.44	179.85	152.02	552.73
SD	9.98	3.98	11.84	9.26	38.90
CV%	4.76	6.28	6.58	6.09	7.04
n	159	159	160	120	78

SD=Standard Deviation, CV =coefficient of variation, n=Number

## 12.4 Linearity

Two samples were diluted, each in two independent assays, and IGF-I concentration was measured in each dilution. In table 7 the recalculated IGF-I concentrations are shown.

**Table 7** Linearity: recalculated IGF-I concentrations of different diluted samples. The recommended dilution is 1:101.

Dilution:	Sample 1 (calculated, ng/ml)	Sample 1 (calculated, ng/ml)	Dilution:	Sample 2 (calculated, ng/ml)	Dilution:	Sample 2 (calculated, ng/ml)
1:50	480.2	521.8	1:30	161.1	1:25	136.0
1:100	496.6	525.1	1:60	169.8	1:50	142.0
1:200	520.6	507.4	1:120	170.8	1:100	141.7
1:400	531.2	520.0	1:240	174.5	1:200	141.4
1:800	572.0	570.4	1:480	174.7	1:400	134.0
1:1600	604.8	563.2	-	-	-	-

## 12.5 Recovery

Recombinant IGF-I was added in different amounts to human serum. The IGF-I content of the so enriched samples was measured. Results are shown in table 8.

**Table 8** Recovery of recombinant human IGF-I in serum.

added IGF-I [ $\mu\text{g/L}$ ]	IGF-I [ $\mu\text{g/L}$ ]		% recovery	
	100	400		
Sample 1	190	538	106	112
Sample 2	283	623	101	107
Sample 3	265	592	110	110

## 12.6 Trueness / Assay Calibration

Recombinant IGF-I produced by E. coli and of >98% purity (SDS-PAGE, Silverstain) is used as calibrator within the assay. The traceability of this recombinant calibration material to the international reference material of the WHO 02/254 has been proven. Results are published by Burns C et al. in Growth Horm IGF Res. 2009 Oct; 19(5):457-62. Epub 2009 Mar 20. Mediagnost IGF-I RIA is coded by 14a.

The reference material includes 8.5 µg/ampoule IGF-I measured by amino acid analysis and HPLC. Mediagnost IGF-I RIA immunoassay (14a) measures 12.87 µg/ampoule. The mean of all tested immunoassays is 11.61 µg/ampoule.

Thus, Mediagnost results are comparable to other immunological tests for measurement of IGF-I and can easily be transformed to WHO 02/254 by a division with: 1.514.

### **12.7 Cross reactions with animal samples**

Several commercially available animal sera have been used as samples in this assay and therewith it is proven, that the test can be used as heterologous assay for IGF-I measurement in serum samples of primates, rats, mice, cattle, pig, sheep, horse, donkey, goat, dog, cat and guinea pig. Species specific calibration has to be done by the user.

## **13 ASSAY COMPARISON**

Mediagnost IGF-I RIA was compared with two other commercial available assays. Evaluation was conducted by an independent third party and results were published by a peer-reviewed journal (28).

For Research Use Only



## 14 REFERENCES

- 1) Baxter RC. 1986 The somatomedins: insulin-like growth factors. *Adv Clin Chem.*25:49-115
- 2) Daughaday WH, Rotwein P. 1989 Insulin-like growth factors I and II. Peptide, messenger ribonucleic acid and gene structures, serum, and tissue concentrations. *Endocr Rev.* 10:68-91
- 3) Spencer EM (Ed.) 1991 *Modern Concepts of Insulin-Like Growth Factors.* New York: Elsevier.
- 4) Klapper DG, Svoboda ME, Van Wyk JJ. 1983 Sequence analysis of somatomedin-C: confirmation of identity with insulin-like growth factor-I. *Endocrinology.* 112:2215-2217.
- 5) Rinderknecht E, Humbel RE. 1978 The amino acid sequence of human insulin-like growth factor I and its structural homology with proinsulin. *J Biol Chem.* 253:2769-2276.
- 6) Clemmons DR, Van Wyk JJ. 1984 Factors controlling blood concentration of somatomedin C. *Clin Endocrinol Metab.* 13:113-143.
- 7) Ballard J, Baxter R, Binoux M, et al. 1989 On the nomenclature of the IGF binding proteins. *Acta Endocrinol (Copenh).* 121:751-752.
- 8) Drop SLS. 1992 Report on the nomenclature of the IGF binding proteins. *J. Clin Endocrinol Metab.* 74:1215-1216.
- 9) Martin JL, Baxter RC. 1986 Insulin-like growth factor binding protein from human plasma. Purification and characterization. *J Biol Chem.* 261:8754-8760.
- 10) Binkert C, Landwehr J, Mary JL, Schwander J, Heinrich G. 1989 Cloning, sequence analysis and expression of a cDNA encoding a novel insulin-like growth factor binding protein (IGFBP-2). *EMBO J.* 8:2497-2502.
- 11) Furlanetto RW, Underwood LE, Van Wyk JJ, D'Ercole AJ. 1977 Estimation of somatomedin-C levels in normals and patients with pituitary disease by radioimmunoassay. *J. Clin Invest.* 60:648-657.
- 12) Daughaday WH, Kapadia M, Mariz I. 1987 Serum somatomedin binding proteins: physiologic significance and interference in radioligand assay. *J Lab Clin Med.* 109:355-363.
- 13) Breier BH, Gallaher BW, Gluckman PD. 1991 Radioimmunoassay for insulin-like growth factor-I: solutions to some potential problems and pitfalls. *J Endocrinol.* 128:347-357.
- 14) Daughaday WH, Mariz IK, Blethen SL. 1980 Inhibition of access of bound somatomedin to membrane receptor and immunobinding sites: a comparison of radioreceptor and radioimmunoassay of somatomedin in native and acid-ethanol-extracted serum. *J Clin Endocrinol Metab.* 51:781-788.
- 15) Blum WF, Gallaher B, Ranke MB. 1992 An IGFBP-blocked IGF-I RIA that measures what it pretends to measure: IGF-I. 74th Annual Meeting of the American Endocrine Society. 293.
- 16) Rosenfeld RG, Wilson DM, Lee PDK, Hintz RL. 1986 Insulin-like growth factors I and II in evaluation of growth retardation. *J Pediatr.* 109:428-433.
- 17) Clemmons DR, Van-Wyk JJ, Ridgway EC, Kliman B, Kjellberg RN, Underwood LE. 1979 Evaluation of acromegaly by radioimmunoassay of somatomedin-C. *N. Engl J Med.* 301:1138-1142.
- 18) Zapf J, Walter H, Froesch ER. 1981 Radioimmunological determination of insulin-like growth factors I and II in normal subjects and in patients with growth disorders and extrapancreatic tumor hypoglycemia. *J Clin Invest.* 68:1321-1330.
- 19) Blum WF. 1992 Insulin-like growth factors and their binding proteins. In: Ranke MB, ed. *Functional Endocrinologic Diagnostics in Children and Adolescence.* Mannheim: J + J Verlag; 102-117.
- 20) Rieu M, Girard F, Bricaire H, Binoux M. 1982 The importance of insulin-like growth factor (somatomedin) measurements in the diagnosis and surveillance of acromegaly. *J Clin Endocrinol Metab.* 55:147-153.
- 21) Blum WF, Ranke MB, Bierich JR. 1988 A specific radioimmunoassay for insulin-like growth factor II: the interference of IGF binding proteins can be blocked by excess IGF-I. *Acta Endocrinol (Copenh).*118:374-380.
- 22) Wilson EM, Oh Y, Rosenfeld RG (1997) Generation and characterization of an IGFBP-7 antibody: Identification of 31 kD IGFBP-7 in human biological fluids and Hs578T human breast cancer conditioned media. *J Clin Endocrinol Metab* Vol 82, 4:1301-1303.

- 23)** Ranke MB, Schweizer R, Elmlinger MW, Weber K, Binder G, Schwarze CP, Wollmann HA (2000) Significance of basal IGF-I, IGFBP-3 and IGFBP-2 measurements in the diagnostics of short stature in children. *Horm Res* 54:60-68
- 24)** Ranke MB, Schweizer R, Elmlinger MW, Weber K, Binder G, Schwarze CP, Wollmann HA (2001) Relevance of IGF-I, IGFBP-3 and IGFBP-2 measurements during GH treatment of GH-deficient and non-GH-deficient children and adolescents. *Horm Res* 55:155-124
- 25)** Address NIBSC:Blance Lane, South Mimms, Potters Bar, Hertford EN 6 3 QG, Great Britain
- 26)** Burns C, Rigsby P, Moore M, Rafferty B. (2009) The first International Standard for Insulin-like Growth Factor-1 (IGF-1) for immunoassay: Preparation and calibration in an international collaborative study. *Growth Hormone & IGF Research* (2009)
- 27)** Blum WH, Breier BH (1994) Radioimmunoassays for IGFs and IGFBPs. *Growth Regulation* 4 (Suppl. 1):11-19
- 28)** Ranke MB, Osterziel KJ, Schweizer R, Schuett B., Weber K., Röbbel P, Vornwald A, Blumenstock G, Elmlinger MB (2003) Reference Levels of Insulin-Like-Growth Factor I in the Serum of Healthy Adults: Comparison of Four Immunoassays. *Clin Chem Lab Med* Vol 41(10):1329-1334

For Research Use Only

For Research Use Only

## 15 ASSAY PROCEDURE

Reagent preparation:		Reconstitution:	Dilution:
<b>B</b>	<b>1. Antibody</b>	in <b>11 mL Assay Buffer A</b>	-
<b>C</b>	<b>Tracer</b>	in <b>11 mL Assay Buffer A</b>	-
<b>D</b>	<b>NSB</b>	in <b>500 µL Assay Buffer A</b>	-
<b>E-L</b>	<b>Calibrators</b>	in <b>500 µL Dilution Buffer DB</b>	-
<b>M+N</b>	<b>Controls</b>	in <b>100 µL Aqua dest.</b>	<b>1:101 with DB</b>
<b>O</b>	<b>2. Antibody</b>	in <b>1 mL Assay Buffer A</b> <b>Mix</b> immediately before use with <b>55 mL Reagent P (1:56)</b>	

Dilute **Samples** with Dilution Buffer **DB 1:101**.

Before use, all kit components, except Reagent **P**, should be brought to room temperature at **20 - 25 °C (68 - 77 °F)**.

### Assay procedure for double determination

Nr. of Tubes	Contents of Tubes	DB, E-L M, N Samples	D (NSB)	B (1.Antibody)	C (Tracer)
<b>1 / 2</b>	Total Counts	-	-	-	100 µL
<b>3 / 4</b>	NSB	100 µL <b>DB</b>	100 µL	-	100 µL
<b>5 / 6</b>	B0	100 µL <b>E</b>	-	100 µL	100 µL
<b>7 - 20</b>	Calibrators	100 µL <b>F-L</b>	-	100 µL	100 µL
<b>21 / 22</b>	High Control	100 µL <b>M</b>	-	100 µL	100 µL
<b>23 / 24</b>	Low Control	100 µL <b>N</b>	-	100 µL	100 µL
<b>25 / 26</b>	Sample 1	100 µL	-	100 µL	100 µL
<b>27 / 28</b>	Sample 2	100 µL	-	100 µL	100 µL
<b>etc.</b>					
<b>Colour after addition</b>		Green	Blue		Violet

Nr.: 1, 2 remove until counting the activity.

**Mix** other tubes with a Vortex-Mixer.

**Incubation at 2 - 8 °C (35.6 - 46.4 °F), at least 40 hours (max. 92 hours)**

Add **500 µL P** (after addition of reagent **O**) in all Tubes  
The reagent-mix should be cold **2 - 8 °C (35.6 - 46.4 °F)**

**Mix** with Vortex-Mixer.

**Incubation at 2 - 8 °C (35.6 - 46.4 °F), 1 h**

**Add 1 mL ice-cold A. dest.**

**Centrifugation at ≥ 3000 x g, 30 min, 2 - 8 °C (35.6 - 46.4 °F)**

Aspirate the supernatant  
(as a precaution, e.g. leave approx. 2 mm as a remaining supernatant above the precipitate).

**Count** the activity of all tubes with a Gamma Counter.